

DC Electronic Load

PEL-3000

PROGRAMMING MANUAL

VERSION: 1.40



ISO-9001 CERTIFIED MANUFACTURER

GW INSTEK

This manual contains proprietary information, which is protected by copyright. All rights are reserved. No part of this manual may be photocopied, reproduced or translated to another language without prior written consent of Good Will company.

The information in this manual was correct at the time of printing. However, Good Will continues to improve products and reserves the rights to change specification, equipment, and maintenance procedures at any time without notice.

Good Will Instrument Co., Ltd.
No. 7-1, Jhongsing Rd., Tucheng Dist., New Taipei City 236, Taiwan.

Table of Contents

I INTERFACE OVERVIEW	2
Front Panel Overview	3
Rear Panel Overview	4
Interface Configuration	5
C COMMAND OVERVIEW	16
Command Syntax	16
Command List	21
Status Registers	154
Error Messages	163


INTERFACE OVERVIEW

This chapter describes basic configuration of IEEE488.2 based remote control.

Front Panel Overview	3
Rear Panel Overview.....	4
Interface Configuration	5
Configure to USB Remote Interface	5
Configure GPIB Interface	6
Configure RS232C	7
RS232C/USB Remote Control Function Check.....	8
Using Realterm to Establish a Remote Connection.....	9
GPIB Function Check.....	13


Front Panel Overview

(PEL-3021/PEL-3041 shown)

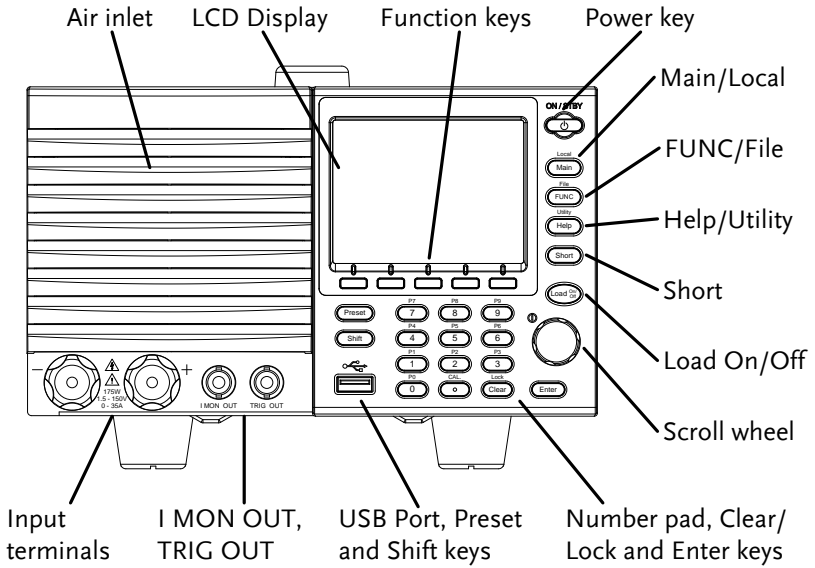

Rear Panel Overview

(PEL-3021 / PEL-3041 shown)

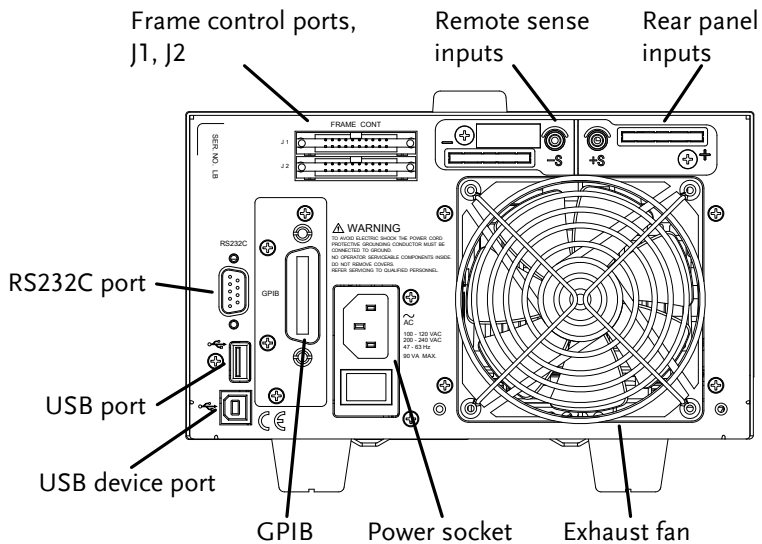

Interface Configuration



Configure to USB Remote Interface

USB configuration	PC side connector	Type A, host
	PEL-3000 side connector	Rear panel Type B, slave
	Speed	2.0 (full speed)
	USB Class	USB CDC AMC



Note

Before USB can be used for remote control, it is necessary to install the PEL-3000 USB device driver, located on the accompanying User Manual CD.

- Operation
1. Connect the USB cable to the rear panel USB B port.
 2. Press  +  > *Interface*[F3] and set the *Interface* setting to *USB*.


Configure GPIB Interface

To use GPIB, the optional GPIB port must be installed. See the user manual for details.

- Operation
1. Ensure the PEL-3000 is off before proceeding.
 2. Connect a GPIB cable from a GPIB controller to the GPIB port on the PEL-3000.
 3. Turn the PEL-3000 on.
 4. Press **Shift** + **Utility Help** > *Interface[F3]* and set the *Interface* setting to *GPIB*.
 5. Set the GPIB address.
 GPIB address 0~30

- GPIB constraints
- *Maximum 15 devices altogether, 20m cable length, 2m between each device*
 - *Unique address assigned to each device*
 - *At least 2/3 of the devices turned On*
 - *No loop or parallel connection*

Pin Assignment



Pin	Signal	Pin	Signal
1~4	Data I/O 1~4	13~16	Data I/O 5~8
5	EOI	17	REN
6	DAV	18	Ground (DAV)
7	NRFD	19	Ground (NRFD)
8	NDAC	20	Ground (NDAC)
9	IFC	21	Ground (IFC)
10	SRQ	22	Ground (SRQ)

11	ATN	23	Ground (ATN)
12	SHIELD Ground	24	Single GND

Configure RS232C


RS232C Configuration	Connector	DB-9, Male
	Baud Rate	2400, 4800, 9600, 19200, 38400
	Stop Bit	1, 2
	Parity	None, Odd, Even

Operation 1. Connect an RS232C cable from the PC to the rear panel RS232 port.

2. Press **Shift** + **Help** > *Interface*[F3] and set the *Interface* setting to RS232.


3. Set the *Baud Rate*, *Stop Bit* and *Parity* settings.

Pin Assignment



- 2: RxD (Receive data)
- 3: TxD (Transmit data)
- 5: GND
- 4, 6 ~ 9: No connection

PC Connection Use a null modem connection as shown in the diagram below.

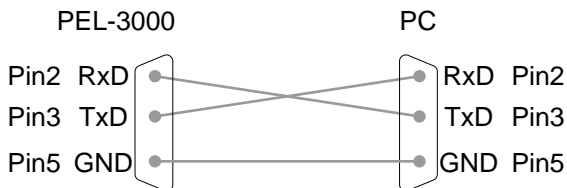

RS232C/USB Remote Control Function Check

Functionality
check

Invoke a terminal application such as RealTerm. For RS232C, set the COM port, baud rate, stop bit, data bit and parity accordingly.

To check the COM settings, see the Device Manager in the PC. For WinXP; Control panel → System → Hardware tab.

Run this query command via the terminal after the instrument has been configured for RS232/USB remote control (page 5).

*idn?

This should return the Manufacturer, Model number, Serial number, and Firmware version in the following format.

- *GW-INSTEK, PEL-3000, XXXXXXXXXXXXX, V.X.X.X*

Manufacturer: GW-INSTEK

Model number : PEL-3000

Serial number : XXXXXXXXXXXXX

Firmware version : V.X.X.X

Using Realterm to Establish a Remote Connection

Background Realterm is a terminal program that can be used to communicate with a device attached to the serial port of a PC or via an emulated serial port via USB.

The following instructions apply to version 1.99.0.27. Even though Realterm is used as an example to establish a remote connection, any terminal program can be used that has similar functionality.



Note


Realterm can be downloaded on Sourceforge.net free of charge.

For more information please see <http://realterm.sourceforge.net/>

- Operation**
1. Download Realterm and install according to the instructions on the Realterm website.
 2. Connect the PEL-3000 via USB (page 5) or via RS232 (page 7).
 3. If using RS232, make note of the configured baud rate, stop bits and parity.
 4. Go to the Windows device manager and find the COM port number for the connection. For example, go to the Start menu > Control Panel > Device Manager

Double click the *Ports* icon to reveal the connected serial port devices and the COM port for the each connected device.

If using USB, the baud rate, stop bit and parity settings can be viewed by right-clicking the connected device and selecting the *Properties* option.

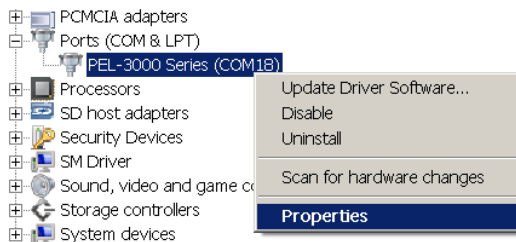

5. Start Realterm on the PC as an administrator.
Click:
Start menu>All Programs>RealTerm>realterm


Tip: to run as an administrator, you can right click the Realterm icon in the Windows Start menu and select the *Run as Administrator* option.

6. After Realterm has started, click on the *Port* tab.

Enter the *Baud*, *Parity*, *Data bits*, *Stop bits* and *Port* number configuration for the connection.

The *Hardware Flow Control*, *Software Flow Control* options can be left at the default settings.

Press *Open* to connect to the PEL-3000.

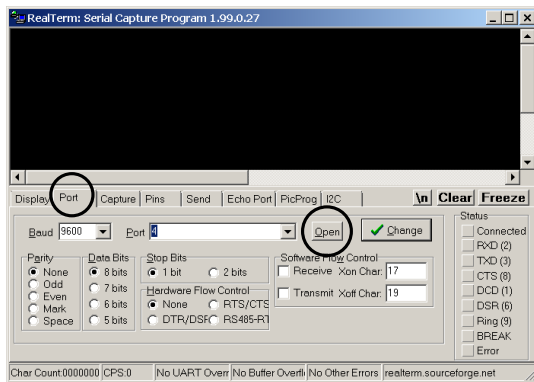


- Click on the *Send* tab.

In the *EOL* configuration, check on the *+CR* and *+LF* check boxes.

Enter the query:
**idn?*

Click on *Send ASCII*.

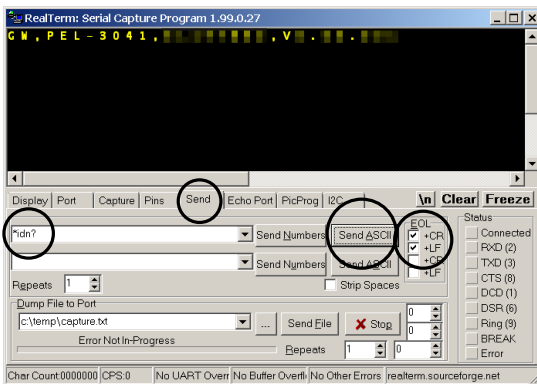

- The terminal display will return the following:

GW, PEL-3XXX,EXXXXXXXXX,VX.XX.XXX

(manufacturer, model, serial number, version)

- If Realterm fails to connect to the PEL-3000, please check all the cables and settings and try again.

GPIB Function Check

Functionality
check

Please use the National Instruments Measurement & Automation Controller software to confirm GPIB/LAN functionality.


See the National Instrument website,
<http://www.ni.com> for details.

Operation

1. Start the NI Measurement and Automation Explorer (MAX) program. Using Windows, press:




*Start>All Programs>National
Instruments>Measurement & Automation*

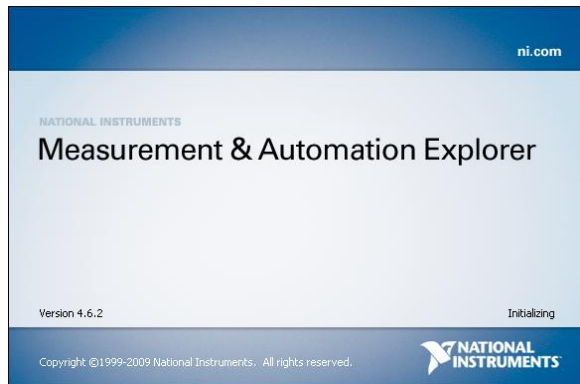

2. From the Configuration panel access;
My System>Devices and Interfaces>GPIB0

3. Press the *Scan for Instruments* button.
4. In the *Connected Instruments* panel the PEL-3000 should be detected as *Instrument 0* with the address the same as that configured on the PEL-3000.
5. Double click the *Instrument 0* icon.

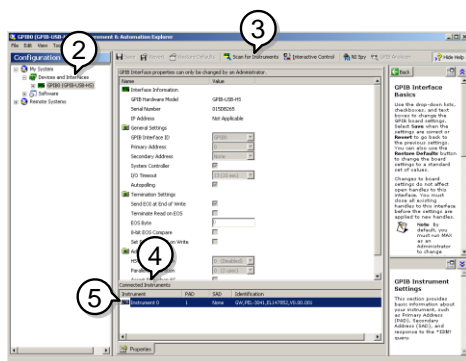


6. Click on *Communicate with Instrument*.
7. In the *NI-488.2 Communicator* window, ensure **IND?* is written in the *Send String:* text box.

Click on the *Query* button to send the **IDN?* query to the instrument.

8. The *String Received* text box will display the query return:

GW, PEL-3XXX, EXXXXXXXX, VX.XX.XXX
 (manufacturer, model, serial number, version)

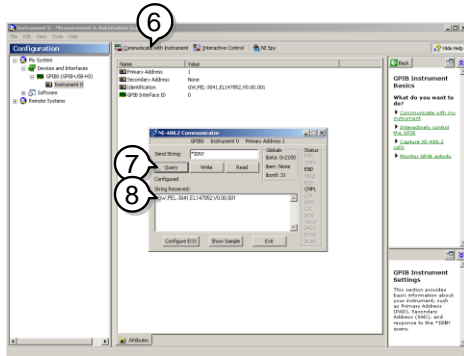

9. The function check is complete.

C COMMAND OVERVIEW

The Command overview chapter lists all PEL-3000 commands in functional order as well as alphabetical order. The command syntax section shows you the basic syntax rules you have to apply when using commands.

Command Syntax

Compatible
Standard

IEEE488.2

Partial compatibility


SCPI, 1999

Partial compatibility

Command
Structure

SCPI (Standard Commands for Programmable Instruments) commands follow a tree-like structure, organized into nodes. Each level of the command tree is a node. Each keyword in a SCPI command represents each node in the command tree. Each keyword (node) of a SCPI command is separated by a colon (:).

For example, the diagram below shows an SCPI sub-structure and a command example.

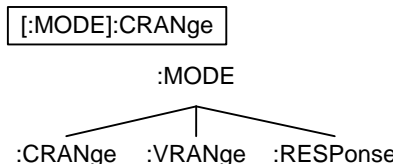

Command types There are a number of different instrument commands and queries. A command sends instructions or data to the unit and a query receives data or status information from the unit.

Command types

Simple A single command with/without a parameter

Example :CONFigure:RESPonse MAX

Query A query is a simple or compound command followed by a question mark (?). A parameter (data) is returned.

Example :CONFigure:RESPonse?

Compound Two or more commands on the same command line. Compound commands are separated with either a semi-colon (;) or a semi-colon and a colon (;:).

A semi-colon is used to join two related commands, with the caveat that the last command must begin at the last node of the first command.

A semi-colon and colon are used to combine two commands from different

nodes.

Example	CONFigure:VON MAX;:CONFigure:VDElay MIN
---------	---

Command Forms Commands and queries have two different forms, long and short. The command syntax is written with the short form of the command in capitals and the remainder (long form) in lower case.

The commands can be written in capitals or lower-case, just so long as the short or long forms are complete. An incomplete command will not be recognized.


Below are examples of correctly written commands.

Long form	:CURRent:LEVel? :CURRENT:LEVEL? :current:level?
Short form	:CURR:LEV? :curr:lev?

Square Brackets Commands that contain square brackets indicate that the contents are optional. The function of the command is the same with or without the square bracketed items, as shown below

For example for the query:
“[:CONFigure]:GNG [:PASS]?”

Both “:CONFigure:GNG:PASS?” and “:GNG?” are both valid forms.

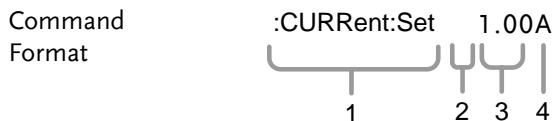

1. Command header
2. Space
3. Parameter 1
4. Unit or suffix.

Common Unit Parameters	Type	Description	Example
	<Boolean>	boolean logic	0, 1
	<NR1>	integers	0, 1, 2, 3
	<NR2>	decimal numbers	0.1, 3.14, 8.5
	<NR3>	floating point	4.5e-1, 8.25e+1
	<NRf>	any of NR1, 2, 3	1, 1.5, 4.5e-1
	[MIN] (Optional parameter)	For commands, this will set the setting to the lowest value. This parameter can be used in place of any numerical parameter where indicated. For queries, it will return the lowest possible value allowed for the particular setting.	
	[MAX] (Optional parameter)	For commands, this will set the setting to the highest value. This parameter can be used in place of any numerical parameter where indicated. For queries, it will return the highest possible value allowed for the particular setting.	
	Unit Suffixes (Optional parameters)	Unit suffixes can be optionally used with most NRf type input parameters.	

[A]	Amps	1.00A
[%]	Percentage	10%
[V]	Volts	5.00V
[W]	Watts	3.00W
[ms]	milliseconds	20ms
[mV]	Millivolts	150mV
[s]	Seconds	5s
[mS]	Reciprocal of 1000 ohms	20mS
[OHM]	Ohm	50OHM
[mA/us]	Millamps/ microsecond	100mA/us
[Hz]	Hertz	1000Hz
Note:	For [OHM] return values, an infinite resistance (open) will be returned as 9.9e ³⁷ .	

Message Terminator	LF	Line feed code (0x0A)
--------------------	----	-----------------------

Command List

Common Commands	*CLS	27
	*ESE	27
	*ESR?	28
	*IDN?	28
	*OPC	29
	*RCL	29
	*RST	29
	*SAV	30
	*SRE	30
	*STB?	31
	*TRG	31
	*TST?	32
	*WAI	32
Trigger Commands	:ABORt	33
	:INPut[:STATe]:TRIGgered	34
	:INITiate[:IMMEdiate]	34
	:INITiate:CONTInuous	34
	:CONDuctance[:VA]:TRIGgered	35
	:CURRent[:VA]:TRIGgered	35
	:RESistance[:VA]:TRIGgered	36
Input State Commands	:INPut	37
	:INPut:SHORT	37
	:INPut:MODE	38
Measurement Commands	:MEASure:CURRent?	39
	:MEASure:VOLTage?	39
	:MEASure:POWer?	39
	:MEASure:ETIME?	40
Configure Subsystem Commands	[:CONFIgure]:OCP	41
	[:CONFIgure]:OPP	42
	[:CONFIgure]:UVP	43
	[:CONFIgure]:OVP	43

	[:CONFigure]:SStart.....	44
	[:CONFigure]:VON.....	45
	[:CONFigure]:VDElay.....	45
	:CONFigure:RESPOse	46
	[:CONFigure]:CNTime	46
	[:CONFigure]:COTime	47
	[:CONFigure]:CRUNit.....	48
	:CONFigure:DYNamic.....	48
	:CONFigure:MEMory.....	49
	:CONFigure:SHORt.....	49
	[:CONFigure]:GNG:SPEctest.....	50
	[:CONFigure]:GNG:DTIME	50
	[:CONFigure]:GNG:MODE	51
	[:CONFigure]:GNG[:PASS].....	51
	[:CONFigure]:GNG:H.....	52
	[:CONFigure]:GNG:L.....	52
	[:CONFigure]:GNG:C	53
Parallel	[:CONFigure]:PARAllel	54
Commands		
Step Commands	[:CONFigure]:STEP:CCH.....	56
	[:CONFigure]:STEP:CCM.....	57
	[:CONFigure]:STEP:CCL.....	57
	[:CONFigure]:STEP:CC	58
	[:CONFigure]:STEP:CRH.....	58
	[:CONFigure]:STEP:CRM.....	59
	[:CONFigure]:STEP:CRL.....	60
	[:CONFigure]:STEP:CR	60
	[:CONFigure]:STEP:CVH.....	61
	[:CONFigure]:STEP:CVL.....	61
	[:CONFigure]:STEP:CV	62
	[:CONFigure]:STEP:CPH.....	62
	[:CONFigure]:STEP:CPM.....	63
	[:CONFigure]:STEP:CPL.....	63
	[:CONFigure]:STEP:CP.....	64
External	[:CONFigure]:EXTernal[:CONTRol].....	65
Commands	[:CONFigure]:EXTernal:LOADonin	65

Mode Subsystem	:MODE.....	67
Commands	[:MODE]:CRANge.....	67
	[:MODE]:VRANge.....	68
	[:MODE]:RESPonse.....	68
	[:MODE]:DYNamic.....	69
Current	:CURRent[:VA]	70
Subsystem	:CURRent:VB	71
Commands	:CURRent:SRATe	71
	:CURRent:L1	72
	:CURRent:L2	72
	:CURRent:SET	73
	:CURRent:LEVel	74
	:CURRent:RISE	74
	:CURRent:FALL	75
	:CURRent:T1	75
	:CURRent:T2	76
	:CURRent:FREQuency.....	77
	:CURRent:DUTY.....	77
Resistance	:CONDuctance[:VA].....	79
Subsystem	:CONDuctance:VB.....	80
Commands	:RESistance[:VA].....	81
	:RESistance:VB.....	81
	:RESistance:SRATe.....	82
	:CONDuctance:L1.....	83
	:CONDuctance:L2.....	83
	:CONDuctance:SET	84
	:RESistance:L1	85
	:RESistance:L2.....	86
	:RESistance:SET	86
	:RESistance:LEVel.....	87
	:RESistance:RISE.....	88
	:RESistance:FALL.....	88
	:RESistance:T1.....	89
	:RESistance:T2.....	89
	:RESistance:FREQuency	90
	:RESistance:DUTY.....	91
	Voltage Subsystem Commands	92
	:VOLTag[:VA]	92
	:VOLTag:VB.....	92

Voltage	:VOLTage[:VA]	92
Subsystem	:VOLTage:VB	92
Commands		
Power Subsystem	:POWer[:VA].....	94
Commands	:POWer:VB	95
	:POWer:L1	95
	:POWer:L2	96
	:POWer:SET	96
	:POWer:LEVel	97
	:POWer:T1	98
	:POWer:T2	98
	:POWer:FREQuency.....	99
	:POWer:DUTY.....	100
Function	:PROGram:STATe	102
Commands	:PROGram	103
	:PROGram[:RECall]:DEFault	104
	:PROGram:STARt	104
	:PROGram:STEP.....	105
	:PROGram:MEMory.....	105
	:PROGram:RUN.....	105
	:PROGram:ONTime.....	106
	:PROGram:OFFTime	106
	:PROGram:PFTime	107
	:PROGram:STIME	107
	[:PROGram]:CHAI:n:STARt	108
	[:PROGram]:CHAI:n.....	108
	[:PROGram]:CHAI:n:P2P	110
	[:PROGram]:CHAI:n[:RECall]:DEFault.....	110
	:PROGram:SAVE.....	111
	:NSEquence:STATe	111
	:NSEquence	112
	:NSEquence:STARt.....	113
	:NSEquence:NUMBER	114
	:NSEquence:MEMO	114
	:NSEquence:MODE	115
	:NSEquence:RANGe	115
	:NSEquence:LOOP.....	116
	:NSEquence:LLOad	116

	:NSEquence:LAST	117
	:NSEquence:CHAIIn	117
	:NSEquence:EDIT	118
	:NSEquence:EDIT:POINt	119
	:NSEquence:EDIT:END?	120
	:NSEquence[:DELet]:ALL	120
	:NSEquence:SAVE	120
	:FSEquence:STATe	120
	:FSEquence	121
	:FSEquence:MEMO	122
	:FSEquence:MODE	123
	:FSEquence:RANGe	123
	:FSEquence:LOOP	124
	:FSEquence:TBASE	124
	:FSEquence:LLOad	125
	:FSEquence:LAST	125
	:FSEquence:RPTStep	126
	:FSEquence:EDIT	126
	:FSEquence:EDIT:POINt	127
	:FSEquence:EDIT:END?	128
	:FSEquence[:DELet]:ALL	128
	:FSEquence[:EDIT]:FILL	128
	:FSEquence:SAVE	129
Utility	:UTILity:SYSTem?	130
Commands	:UTILity:LOAD	131
	:UTILity:LOAD:MODE	132
	:UTILity:LOAD:RANGe	132
	:UTILity:INTerface	133
	:UTILity:BRATe	133
	:UTILity:SBIT	134
	:UTILity:PARity	134
	:UTILity:TIME	135
	:UTILity:KNOB	135
	:UTILity:SPEaker	136
	:UTILity:ALARm	136
	:UTILity:UNReg	137
	:UTILity:GNG	137
	:UTILity:CONTRast	138
	:UTILity:BRIGhtness	138
	:UTILity:LANGUage	138
	:UTILity:REMOte	139
	:UTILity:REMOte:MODE	139

File Commands	:MEMory:SAVE.....	140
	:MEMory:RECall.....	140
	:PRESet:SAVE.....	141
	:PRESet:RECall	141
	:SETup:SAVE.....	141
	:SETup:RECall	141
	:FACTory[:RECall]	142
	:USER[:DEFault]:SAVE.....	142
:USER[:DEFault]:RECall.....	142	
SCPI Register Commands	:SYSTem:ERRor?.....	143
	:STATus:PRESet	144
	:STATus:QUEStionable:CONDition?	144
	:STATus:QUEStionable:ENABLE	145
	:STATus:QUEStionable[:EVENT]?	145
	:STATus:QUEStionable:NTRansition	146
	:STATus:QUEStionable:PTRansition	147
	:STATus:OPERation:CONDition?	147
	:STATus:OPERation:ENABLE	148
	:STATus:OPERation[:EVENT]?.....	148
	:STATus:OPERation:NTRansition	149
	:STATus:OPERation:PTRansition	149
	:STATus:CSUMmary:CONDition?	150
	:STATus:CSUMmary:ENABLE	150
	:STATus:CSUMmary[:EVENT]?.....	151
:STATus:CSUMmary:NTRansition	151	
:STATus:CSUMmary:PTRansition	152	

Common Commands


*CLS	27
*ESE	27
*ESR?	28
*IDN?	28
*OPC	29
*RCL	29
*RST	29
*SAV	30
*SRE	30
*STB?	31
*TRG	31
*TST?	32
*WAI	32

*CLS



Description Clears the error queue.

Syntax *CLS



*ESE



Description Queries or sets the Standard Event Status Enable register. The Standard Event Status Enable register determines which events can set the Event Summary bit (ESB) in the Status Byte Register. Any bits that are set to 1 enable the corresponding event. Each event is represented by a bit in the Standard Event Status Enable register.

Syntax *ESE <NR1>

Query Syntax *ESE?

Parameter/ Return parameter	<NR1> (bit weight)	Bit number / Description
	1	0/ OPC
	4	2/ QYE
	8	3/ DDE

16	4/ EXE
32	5/ CME

Example *ESE 8
Sets bit 3 of the ESE register.

Query example *ESE?
>12
Bits 2 and 3 are set in the Standard Event Status Enable register.

***ESR?** → Query

Description Reads the Standard Event Status register. This command will also clear the Standard Event Status register.

Query Syntax *ESR?

Return parameter	<NR1> (bit weight)	Bit number / Description
	4	3/ QYE
	8	4/ DDE
	16	5/ EXE
	32	6/ CME

Query example *ESR?
>48
Bits 4 and 5 are set in the Standard Event register.

***IDN?** → Query

Description Queries the manufacturer, model number, serial number, and firmware version of the instrument.

Query Syntax *IDN?

Return parameter <string> Returns the instrument identification as a string in the following format:
GW-INSTEK, PEL-3021, XXXXXXXX, V.VV
Manufacturer: GWINSTEK
Model number : PEL-3021
Serial number : XXXXXXXX
Firmware version : V.VV

Set →

← Query

***OPC**

Description This command sets the OPC (Operation Command Bit) bit (bit 0) of the Standard Event Status Register after the instrument has completed all pending operations. The query will return the status of the OPC bit.

Syntax *OPC

Query Syntax *OPC?

Return parameter <NR1>
 1 Operation complete

Query Example *OPC?
 >1
 Indicates that all pending operations are complete.

***RCL**

Set →

Description The Recall Instrument State command restores the instrument settings from a previously saved memory setting.

Syntax *RCL <NR1>

Parameter <NR1>
 1~256 Memory number 1 to 256

Example *RCL 20
 Recall setting memory 20.

***RST**

Set →

Description Resets the unit. This is command forces the ABORT, and *CLS

Syntax *RST

***SAV**

Set →

Description	The Save Instrument State command saves the instrument settings to one of the memory setting slots.	
Syntax	*SAV <NR1>	
Parameter	<NR1> 1~256	Memory number 1 to 256
Example	*SAV 20 Saves the current setting to memory 20.	

Set →

***SRE**

→ Query

Description	Queries or sets the Service Request Enable register. The Service Request Enable register determines which events in the Status Byte register can set the Master Summary bit (MSB) in the Status Byte Register. Any bits that are set to 1 will cause the MSS bit to be set.	
Syntax	*SRE <NR1>	
Query Syntax	*SRE?	
Parameter/ Return parameter	<NR1> (bit weight)	Bit number / Description
	1	0/Not used
	2	1/ERR
	4	2/ CSUM
	8	3/ QUES
	16	4/ MAV
	32	5/ ESB
	64	6/ RQS_MSS
	128	7/ OPER
	Note: Bit 1 and 2 cannot be set, however bit 1 (ERR) can be returned.	
Example	*SRE 8 Sets bit 3 of the Service Request Enable register.	

Query example *SRE?
 >12

Bits 2 and 3 are set in the Service Request Enable register.

***STB?** → Query

Description Reads the Status Byte register. This command will not clear the Status Byte register.

If the Master Summary Status bit (MSS) is set, it indicates that there is a reason for a service request.

Query Syntax *STB?

Return parameter	<NR1> (bit weight)	Bit number / Description
	1	0/Not used
	2	1/ERR
	4	2/ CSUM
	8	3/ QUES
	16	4/ MAV
	32	5/ ESB
	64	6/ RQS_MSS
	128	7/ OPER

Note: Bit 1 and 2 cannot be set, however bit 2 (ERR) can be returned.

Query example *STB?
 >36

Bits 2 and 5 are set in the Status Byte register.

***TRG** Set →

Description This command triggers the unit.

Syntax *TRG

***TST?**

→ **Query**

Description	This command is a standard SCPI self-test command. The PEL-3000 does not perform any self-tests so will always return 0 (pass) for this command.	
Query Syntax	*TST?	
Return parameter	<NR1> 0	Pass
Query example	*TST? >0	

***WAI**


Set →

Description	Wait command. Prevents new operations from executing until all pending operations have finished.	
Syntax	*WAI	

Trigger Commands

:ABORt	33
:INPut[:STATe]:TRIGgered	34
:INITiate[:IMMediate]	34
:INITiate:CONTinuous	34
:CONDuctance[:VA]:TRIGgered	35
:CURRent[:VA]:TRIGgered	35
:RESistance[:VA]:TRIGgered	36

Trigger States

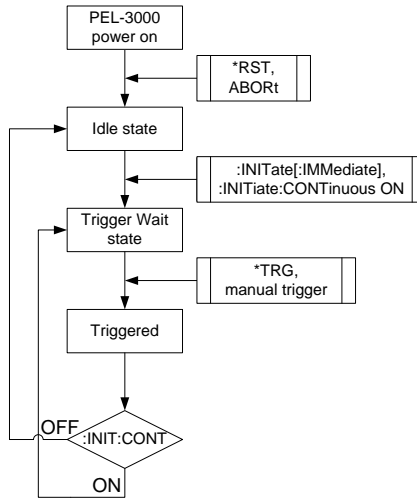



:ABORt

Set →

Description Clears the trigger wait status and returns to the idle state.

Query Syntax :ABORt

:INPut[:STATe]:TRIGgered





Description	Turn ON/OFF the trigger input.	
Syntax	:INPut[:STATe]:TRIGgered {<Boolean> OFF ON }	
Query Syntax	:INPut[:STATe]:TRIGgered?	
Parameter	OFF or 0	Trigger input = OFF
	ON or 1	Trigger input = ON
Return parameter	0	Trigger input = OFF
	1	Trigger input = ON
Example	:INPut:TRIGgered ON Turns the on the trigger input.	
Query example	:INPut:TRIGgered? >0 Indicates that the trigger input is turned off.	

:INITiate[:IMMediate] 

Description	Sets the trigger to the wait state. If the trigger is activated, the trigger will automatically go to the idle state.	
Query Syntax	:INITiate[:IMMediate]	

:INITiate:CONTInuous

Description	Sets or queries whether the trigger will go back to the wait state or go to the idle state after a trigger. When the :INITiate:CONTInuous function is set to OFF, the trigger state can only be returned to idle if the *RST or ABORt command is used	
Syntax	:INITiate:CONTInuous {<Boolean> OFF ON }	
Query Syntax	:INITiate:CONTInuous?	
Parameter	OFF or 0	Continuous = OFF
	ON or 1	Continuous = ON

Return parameter	0	Continuous = OFF
	1	Continuous = ON

Example :INITiate:CONTInuous ON
 Configures the trigger to go to the wait state after a trigger.

Query example :INITiate:CONTInuous?
 >1
 Indicates that the trigger will to go to the wait state after a trigger.

:CONDuctance[:VA]:TRIGgered Set →

Description Sets the conductance value for when the trigger is activated.

Syntax :CONDuctance[:VA]:TRIGgered {<NR2>[mS] |MINimum | MAXimum }

Parameter	<NR2>[mS]	Conductance in millisiemens(mS).
	MINIMUM or MIN	MINIMUM value.
	MAXIMUM or MAX	MAXIMUM value.

Example :CONDuctance:TRIGgered MAX
 Sets the conductance to the maximum value.

:CURRent[:VA]:TRIGgered Set →

Description Sets the current generated when the trigger is activated.

Syntax :CURRent[:VA]:TRIGgered {<NR2>[A] |MINimum | MAXimum }

Parameter	<NR2>[A]	Current in amps.
	MINIMUM or MIN	MINIMUM value.
	MAXIMUM or MAX	MAXIMUM value.

Example :CURRent:TRIGgered MAX
 Sets the current generated to the maximum value.

:RESistance[:VA]:TRIGgered

Set →

Description	Sets the resistance for when the trigger is activated.	
Syntax	:RESistance[:VA]:TRIGgered {<NR2>[OHM] MINimum MAXimum }	
Parameter	<NR2>[OHM] MINIMUM or MIN MAXIMUM or MAX	Resistance in ohms. MINIMUM value. MAXIMUM value.
Example	:RESistance:TRIGgered MAX Sets the resistance to the maximum value.	

Input State Commands

:INPut	37
:INPut:SHORT.....	37
:INPut:MODE	38

:INPut

Set →

→ Query

Description	Sets or queries the status of the load.	
Syntax	:INPut {<Boolean> OFF ON }	
Query Syntax	:INPut?	
Parameter	OFF or 0 ON or 1	Load = OFF Load = ON
Return parameter	0 1	Load = OFF Load = ON
Example	:INPut ON Turns the load on.	
Query example	:INPut? >0 Indicates that the load is off.	

Set →


→ Query

:INPut:SHORT

Description	Shorts or opens the input terminals or queries their status.	
Syntax	:INPut:SHORT {<Boolean> OFF ON }	
Query Syntax	:INPutSHORT?	
Parameter	OFF or 0 ON or 1	Short = OFF Short = ON
Return parameter	0 1	Short = OFF Short = ON
Example	:INPut:SHORT ON Shorts the input terminals.	

Query example :INPut:SHORT?
 >0
 Indicates that the short function is off.

:INPut:MODE



Description	Selects the load function mode.	
Syntax	:INPut:MODE{ LOAD PROG NSEQ FSEQ }	
Query Syntax	:INPut:MODE?	
Parameter/ Return parameter	LOAD	Sets the load to generator as a CC/CV/CP/CR load.
	PROG	Sets the function mode to program.
	NSEQ	Sets the function mode to Normal Sequence mode.
	FSEQ	Sets the function mode to Fast Sequence mode.
Example	:INPut:MODE PROG	Puts the load generator into Program mode.
Query example	:INPut:MODE? >PROG	Indicates that the current function mode is Program.

Measurement Commands

:MEASure:CURRent?	39
:MEASure:VOLTage?	39
:MEASure:POWer?	39
:MEASure:ETIMe?	40

:MEASure:CURRent? → Query

Description	This command returns the load current.	
Query Syntax	:MEASure:CURRent?	
Return parameter	<NR2>	Load current in amps
Query example	:MEASure:CURRent? >0.79860	
	Returns the load current in amps.	

:MEASure:VOLTage? → Query

Description	This command returns the load voltage.	
Query Syntax	:MEASure:VOLTage?	
Return parameter	<NR2>	Load voltage in volts
Query example	:MEASure:VOLTage? >1.49900	
	Returns the load voltage in volts.	

:MEASure:POWer? → Query

Description	This command returns the power.	
Query Syntax	:MEASure:POWer?	
Return parameter	<NR2>	Power in watts
Query example	:MEASure:POWer? >1.19695	
	Returns the power in watts.	

:MEASure:ETIMe?

→ Query

Description	Returns the amount of time the load has been on for in seconds (elapsed time).
-------------	--

Query Syntax	:MEASure:ETIMe?
--------------	-----------------

Return parameter	<NR2>	Elapsed time in seconds
------------------	-------	-------------------------

Query example	:MEASure:ETIMe? >316.0
---------------	---------------------------

Returns the elapsed time in seconds.

Configure Subsystem Commands

[:CONFigure]:OCP.....	41
[:CONFigure]:OPP.....	42
[:CONFigure]:UVP.....	43
[:CONFigure]:OVP	43
[:CONFigure]:SStart.....	44
[:CONFigure]:VON	45
[:CONFigure]:VDElay.....	45
:CONFigure:RESPonse	46
[:CONFigure]:CNTime.....	46
[:CONFigure]:COTime.....	47
[:CONFigure]:CRUNit.....	48
:CONFigure:DYNamic.....	48
:CONFigure:MEMory.....	49
:CONFigure:SHORT.....	49
[:CONFigure]:GNG:SPEctest.....	50
[:CONFigure]:GNG:DTIME	50
[:CONFigure]:GNG:MODE.....	51
[:CONFigure]:GNG:[PASS]	51
[:CONFigure]:GNG:H.....	52
[:CONFigure]:GNG:L.....	52
[:CONFigure]:GNG:C.....	53


[:CONFigure]:OCP




Description	Sets or queries the OCP trip settings. The OCP limit can be set to a specific value or the trip setting can be set to either limit the current or to turn the load off.	
Syntax	[:CONFigure]:OCP {<NRf>[A] MINimum MAXimum LIMit LOFF }	
Query Syntax	[:CONFigure]:OCP?	
Parameter	<NRf>[A]	Current limit value.

	MINIMUM or MIN	Minimum current limit value.
	MAXIMUM or MAX	MAXimum current limit value.
	LIMIT or LIM	Limit the load
	LOFF	Turn the load off
Return parameter	Returns a string with OCP setting followed by the OCP value.	
Example1	:OCP LIM	Sets the OCP setting to limit.
Example2	:OCP 77.000	Sets the OCP value to 77A.
Query example	:OCP? >LIMIT, 77.000	The OCP setting is LIMIT and the OCP value is 77.000A.

[[:CONFigure]:OPP



Description	Sets or queries the OPP trip settings. The OPP limit can be set to a specific value or the trip setting can be set to either limit the power or to turn the load off.	
Syntax	[:CONFigure]:OPP {<NRf> [W] MINimum MAXimum LIMit LOFF }	
Query Syntax	[:CONFigure]:OPP?	
Parameter	<NRf>[W] MINIMUM or MIN MAXIMUM or MAX LIMIT or LIM LOFF	Power limit value. MINIMUM power limit value. MAXIMUM power limit value. Limit the load Turn the load off
Return parameter	Returns a string with OPP setting followed by the OPP value.	

Example1	:OPP LIMIT Sets the OCP setting to limit.
Example2	:OPP 10.000 Sets the OPP value to 10W.
Query example	:OPP? >LIMIT, 10.000 The OPP setting is LIMIT and the OPP value is 10.000W.

[[:CONFIgure]:UVP

Set →

→ Query

Description	Sets or queries the UVP trip settings. The UVP can also be cleared with this command.	
Syntax	[:CONFIgure]:UVP {<NRf>[V] MINimum MAXimum }	
Query Syntax	[:CONFIgure]:UVP?	
Parameter	<NRf>[V] MINIMUM or MIN MAXIMUM or MAX	voltage limit value. MINIMUM value. MAXIMUM value.
Return parameter	Returns the UVP level (<NR2>)	

Example1	:UVP 10.00 Sets the UVP setting to 10V.
Query example	:UVP? > 10.0000 The UVP setting is 10.0000V.

[[:CONFIgure]:OVP

Set →

→ Query

Description	Sets or queries the OVP trip settings. The OVP can also be cleared with this command.	
Syntax	[:CONFIgure]:OVP {<NRf>[V] MINimum MAXimum}	

Query Syntax	[:CONFigure]:OVP?	
Parameter	<NRf>[V] MINIMUM or MIN MAXIMUM or MAX	voltage limit value. MINIMUM value. MAXIMUM value.
Return parameter	Returns the OVP level (<NR2>).	
Example1	:OVP 10.00 Sets the OVP setting to 10V.	
Query example	:OVP? > 10.0000 The OVP setting is 10.0000V.	

Set →

← Query

[:CONFigure]:SStart

Description	Sets or queries the Soft Start time setting.	
Syntax	[:CONFigure]:SStart {<NRf>[s] MINimum MAXimum OFF }	
Query Syntax	[:CONFigure]:SStart?	
Parameter	<NRf>[s] MINIMUM or MIN MAXIMUM or MAX OFF	The soft start time in seconds. Minimum time = 0 second Maximum time OFF = 0 second
Return parameter	<NR2> OFF	Returns the soft start time in seconds. Off
Example	:SStart OFF Turns the soft start function off.	
Query example	:SStart? >OFF The soft start function is off.	

[[:CONFIgure]:VON




Description	Sets or queries the Von voltage settings.	
Syntax	[:CONFIgure]:VON {<NRf>[V] MINimum MAXimum LON LOFF }	
Query Syntax	[:CONFIgure]:VON?	
Parameter	{<NRf>[V] MINIMUM or MIN MAXIMUM or MAX LON LOFF	The Von voltage level (default unit is V) Minimum Von voltage level Maximum Von voltage level Latch on Latch off
Return parameter	<ASCII string>	Returns the Von latch settings.
Example	:VON 10.0V Sets the Von voltage to 10.0 volts.	
Query example	:VON? >Latch OFF, 10.000 The Von voltage level is 10V.	

[[:CONFIgure]:VDElay




Description	Sets or queries the Von Delay settings in seconds.	
Syntax	[:CONFIgure]:VDElay {<NRf>[s] MINimum MAXimum OFF }	
Query Syntax	[:CONFIgure]:VDElay?	
Parameter	<NRf>[s] OFF MINIMUM or MIN MAXIMUM or MAX	The delay time in seconds Disable the delay time Minimum delay time Maximum delay time
Return parameter	<NR2>	Returns the delay time in seconds

Example :VDElay 1.5 ms
 Sets the delay time to 1.5ms.
 :VDElay 0.0015 s
 Sets the delay time to 1.5ms.

Query example :VDElay?
 >0.0015
 The delay time is 1.5ms.

Set →

→ Query

:CONFigure:RESPonse

Description Sets or queries the response speed. This is the equivalent to the CC, CR and CP Mode.

Syntax :CONFigure:RESPonse {<NR2> | MINimum | MAXimum }

Query Syntax :CONFigure:RESPonse?

Parameter	<NR2>	0.1, 0.2, 0.5, 1.0 (for CC ,CR or CP mode only)
	MINimum	Minimum response speed
	MAXimum	Maximum response speed

Return Parameter <NR2> 0.1, 0.2, 0.5, 1.0

Example :CONFigure:RESPonse MAX
 Sets the response to the maximum.

Query example :CONFigure:RESPonse?
 >1.0
 Returns the response.

Set →

→ Query

[:CONFigure]:CNTTime


Description Turns the Count Time timer function on or off.

Syntax [:CONFigure]:CNTTime {<Boolean> |OFF | ON }


Query Syntax [:CONFigure]:CNTTime?

Parameter/ Return parameter	OFF or 0 ON or 1	Turns the Count Time timer off. Turns the Count Time timer on
Example	[:CONFigure]:CNTTime ON Turns the Count Time timer on.	
Query example	[:CONFigure]:CNTTime? >ON Count Time is turned on.	

[:CONFigure]:COTime



Description	Sets or queries the load cutoff time. A cutoff time of 0 seconds is the equivalent of disabling the cutoff time.	
Syntax	[:CONFigure]:COTime {<NRf>[s] MINimum MAXimum OFF }	
Query Syntax	[:CONFigure]:COTime?	
Parameter	<NRf>[s] OFF MINIMUM or MIN MAXIMUM or MAX	Cut off time in seconds (1~3599999) Turns the cutoff time off. Sets the cutoff time to the maximum Sets the cutoff time to the minimum
Return parameter	<NR1>	Returns the cutoff time
Example	:COTime MAX Sets the cutoff time to the maximum.	
Query example	:COTime? >3599999 The cutoff time is set to 3599999 seconds.	



[[:CONFigure]:CRUNit

Description	Sets or queries the CR mode setting units.	
Syntax	[:CONFigure]:CRUNit {OHM MHO}	
Query Syntax	[:CONFigure]:CRUNit?	
Parameter/ Return parameter	OHM MHO	Set the units to ohms. Set the units to mho (conductance)
Example	:CRUNit OHM Sets the CR mode units to ohms.	
Query example	:CRUNit? >OHM The CR mode units are ohms.	



:CONFigure:DYNamic

Description	Sets the display units for when dynamic mode switching is used. Units can be selected from Percent and Value. See the user manual for further details. This command will also configure whether to switch between each level using timers or a set duty cycle.	
Syntax	:CONFigure:DYNamic { VALue PERCent TIME FDUTy }	
Query Syntax	:CONFigure:DYNamic?	
Parameter	VALUE or VAL PERCENT or PERC TIME FDUTY or FUDT	Set the units to Value. Set the units to Percent. Use timers for timing. Use duty cycle for timing.
Return parameter	<ASCII string>	Return a string containing the unit mode and the timing mode.
Example	:CONFigure:DYNamic VALue Sets the dynamic mode units to value.	

Query example :CONFigure:DYNamic?
> Value,T1,T2

The dynamic mode becomes a value setup and timer setup.

Set →

→ Query

:CONFigure:MEMory

Description This command configures the how the files are recalled *in local mode* (using the front panel interface). By default when you try to recall a file or setting from memory, a message will appear asking you to press the Enter key to confirm each time you wish to recall. This command enables (SAFety) or disables this feature (DIRect).

Syntax :CONFigure:MEMory {SAFety | DIRect }

Query Syntax :CONFigure:MEMory?

Parameter	SAFETY or SAF DIRECT or DIR	Safety setting. Directly recall the chosen file.
------------------	--------------------------------	---

Return parameter	Safety Direct	Safety setting. Directly setting.
-------------------------	------------------	--------------------------------------

Example :CONFigure:MEMory SAFety
Enables the safety setting.

Query example :CONFigure:MEMory?
>Safety
The safety setting is enabled.

Set →

→ Query

:CONFigure:SHORt

Description Configures the short key.

Syntax :CONFigure:SHORt { TOGGle | HOLD }

Query Syntax :CONFigure:SHORt?

Parameter	HOLD	Sets the button configuration to hold
------------------	------	---------------------------------------

	TOGGLE or TOGG	Sets the button configuration to toggle
Return parameter	Toggle Hold	Toggle Hold
Example	:CONFigure:SHORt TOGGle Sets the Short key configuration to toggle.	
Query example	:CONFigure:SHORt? >Toggle The Short key is configured to toggle.	

(Set) →

→ (Query)

[:CONFigure]:GNG:SPECTest

Description	Enables/Disables Go-NoGo testing (SPEC test = ON/SPEC test = OFF).	
Syntax	[:CONFigure]:GNG:SPECTest {<Boolean> OFF ON }	
Query Syntax	[:CONFigure]:GNG:SPECTest?	
Parameter/ Return parameter	OFF or 0 ON or 1	SPEC test = OFF SPEC test = ON
Example	:GNG:SPECTest ON Turns Go-NoGo testing on.	
Query example	:GNG:SPECTest? >OFF Indicates that Go-NoGo testing is off.	

(Set) →

→ (Query)

[:CONFigure]:GNG:DTIME

Description	Sets or queries the Go-NoGo delay time.	
Syntax	[:CONFigure]:GNG:DTIME {<NRf>[s] MINimum MAXimum }	
Query Syntax	[:CONFigure]:GNG:DTIME?	
Parameter	<NRf>[s] MINimum or MIN MAXimum or MAX	Sets the Go-NoGo delay time in seconds (0.0~1.0) with 0.1 second resolution. Minimum delay time Maximum delay time

Return parameter	<NR2>	Returns the delay time in seconds.
Example	:GNG:DTIME 0.5 Sets the delay time to 0.5 seconds.	
Query example	:GNG:DTIME? >0.5 The delay time is 0.5 seconds.	


[[:CONFIgure]:GNG:MODE (Set) →
→ (Query)

Description	Sets or queries the entry mode for the Go-NoGo settings. The entry mode determines whether the Go-NoGo limits are set as values or as a percentage value from a center reference value.	
Syntax	[:CONFIgure]:GNG:MODE {PERCent VALue }	
Query Syntax	[:CONFIgure]:GNG:MODE?	
Parameter	PERCENT or PERC VALUE or VAL	Sets the entry mode to %. Sets the entry mode to value
Return parameter	Percent Value	% entry mode Value entry mode
Example	:GNG:MODE PERCent Sets the entry mode to %.	
Query example	:GNG:MODE? >Percent The entry mode is %.	

[[:CONFIgure]:GNG[:PASS] → (Query)

Description	Queries the Go-NoGo test result(s). This command can be used for all test modes (CC, CV, CR, CP).	
Query Syntax	[:CONFIgure]:GNG[:PASS]?	
Return parameter	NG GO	No Go (fail) Go (Pass)

Query example :GNG?
 >GO
 Returns the Go-NoGo test result.



[:CONFigure]:GNG:H

Description Sets or queries the high voltage/current limit value. If the entry mode is set to value, the high voltage/current limit value units are in volts/amps. If the entry mode is set to percent, the high voltage/current limit value units are in percent.

Syntax [:CONFigure]:GNG:H <NRf>


Query Syntax [:CONFigure]:GNG:H?

Parameter	<NRf>	Sets the high voltage/current limit value in volts/amps or in percent.
------------------	-------	--

Return parameter	<NR2>	Returns the high voltage/current limit value in volts/amps or as %.
-------------------------	-------	---

Example :GNG:H 100.0
 Sets the high voltage limit value to 100%.

Query example :GNG:H?
 >100.0
 Returns the high voltage limit value as 100.0%.




[:CONFigure]:GNG:L

Description Sets or queries the low voltage/current limit value. If the entry mode is set to value, the low voltage/current limit value units are in volts/amps. If the entry mode is set to percent, the low voltage/current limit value units are in percent.

Syntax [:CONFigure]:GNG:L <NRf>

Query Syntax	[:CONFigure]:GNG:L?	
Parameter	<NRf>	Sets the low voltage/current limit value in volts/amps or in percent.
Return parameter	<NR2>	Returns the low voltage/current limit value in volts/amps or as %.
Example	:GNG:L 10.0 Sets the low voltage limit value to 10%.	

Query example :GNG:L?
>10.0
Returns the low voltage limit value as 10.0%.





[:CONFigure]:GNG:C

Description	Sets or queries the center voltage/current limit value. The center voltage limit value is used as the center reference value when the entry mode is set to percent ([:CONFigure]:GNG:Mode=PERCent).	
Syntax	[:CONFigure]:GNG:C <NRf>	
Query Syntax	[:CONFigure]:GNG:C?	
Parameter	<NRf>	Sets the center voltage/current limit value in volts/amps.
Return parameter	<NR2>	Returns the center voltage/current limit value in volts/amps.
Example	:GNG:C 10.0 Sets the center voltage/current limit value to 10V or A.	

Parallel Commands

[:CONFigure]:PARAllel54


[:CONFigure]:PARAllel		 
Description	Configures the unit for parallel operation, or queries its state. This command configures the unit as a Master or Slave, and configures how many slave units are connected if the unit is configured as a master.	
Note	The booster (PEL-3211) cannot use low current range.	
Syntax	[:CONFigure]:PARAllel { OFF MASTER SLAVE P2 P3 P4 P5 B1 B2 B3 B4 }	
Query Syntax	[:CONFigure]:PARAllel?	
Parameter	P2,P3,P4 or P5	Number of connected slaves
	B1,B2,B3 or B4	Number of connected booster
	OFF	Turn parallel mode off
	MASTER or MAST	Sets the unit to Master
	SLAVE or SLAV	Sets the unit to Slave
Return parameter	<ASCII string>	Returns an ASCII string with the mode of the unit (Master/Slave) and the number of connected devices.
Example	:PARAllel MAST Sets the unit to Master. :PARAllel B2 Configures the unit for use with 2 booster units.	

Query example :PARallel?
 >Mode:Master, Number:2

The unit is set to Master and there are connected slaves.

Step Resolution Commands

[:CONFigure]:STEP:CCH.....	56
[:CONFigure]:STEP:CCM.....	57
[:CONFigure]:STEP:CCL.....	57
[:CONFigure]:STEP:CC.....	58
[:CONFigure]:STEP:CRH.....	58
[:CONFigure]:STEP:CRM.....	59
[:CONFigure]:STEP:CRL.....	60
[:CONFigure]:STEP:CR.....	60
[:CONFigure]:STEP:CVH.....	61
[:CONFigure]:STEP:CVL.....	61
[:CONFigure]:STEP:CV.....	62
[:CONFigure]:STEP:CPH.....	62
[:CONFigure]:STEP:CPM.....	63
[:CONFigure]:STEP:CPL.....	63
[:CONFigure]:STEP:CP.....	64



[:CONFigure]:STEP:CCH

Description Configures the step resolution for CC High Range.
 Note: The step resolution setting will be automatically rounded to the closest multiple of the base resolution.

Syntax [:CONFigure]:STEP:CCH {<NRf>[A] | MINimum | MAXimum }

Query Syntax [:CONFigure]:STEP:CCH?

Parameter	<NRf>[A]	Step resolution.
	MINIMUM or MIN	Minimum step resolution
	MAXIMUM or MAX	Maximum step resolution

Return parameter	<ASCII string>	Returns the range and the step resolution.
-------------------------	----------------	--

Example :STEP:CCH 0.002A
 Sets the step resolution to 0.002A.

Query example :STEP:CCH?
 > CCH:0.002
 Returns the step resolution (0.002A).

Set →

[[:CONFigure]:STEP:CCM

→ Query

Description Configures the step resolution for CC medium Range. Note: The step resolution setting will be automatically rounded to the closest multiple of the base resolution.

Syntax [[:CONFigure]:STEP:CCM {<NRf>[A] | MINimum | MAXimum }

Query Syntax [[:CONFigure]:STEP:CCM?

Parameter	<NRf>[A]	Step resolution.
	MINIMUM or MIN	Minimum step resolution
	MAXIMUM or MAX	Maximum step resolution

Return parameter	<ASCII string>	Returns the range and the step resolution.
-------------------------	----------------	--

Example :STEP:CCM 0.0002A
 Sets the step resolution to 0.0002A.

Query example :STEP:CCM?
 >CCM:0.0002
 Returns the step resolution (0.0002A).

Set →

[[:CONFigure]:STEP:CCL

→ Query

Description Configures the step resolution for CC low Range. Note: The step resolution setting will be automatically rounded to the closest multiple of the base resolution.

Syntax [[:CONFigure]:STEP:CCL {<NRf>[A] | MINimum | MAXimum }

Query Syntax [[:CONFigure]:STEP:CCL?

Parameter	<NRf>[A] MINIMUM or MIN MAXIMUM or MAX	Step resolution. Minimum step resolution Maximum step resolution
Return parameter	<ASCII string>	Returns the range and the step resolution.
Example	:STEP:CCL 0.02mA Sets the step resolution to 0.02mA.	
Query example	:STEP:CCL? > CCL:0.00002 Returns the step resolution (0.00002A).	

[:CONFigure]:STEP:CC → Query

Description	Returns the step resolution for each CC Mode range as a string.	
Query Syntax	[:CONFigure]:STEP:CC?	
Return parameter	<ASCII string>	Returns the CCH, CCM and CCL step resolution settings.
Query example	:STEP:CC? >CCH:0.002, CCM:0.0002, CCL:0.00002 Returns the CC mode step resolution for each range.	

Set →

[:CONFigure]:STEP:CRH → Query

Description	Configures the step resolution for CR High Range. Note: The step resolution setting will be automatically rounded to the closest multiple of the base resolution.	
Syntax	[:CONFigure]:STEP:CRH {<NRf>[mS] MINimum MAXimum }	
Query Syntax	[:CONFigure]:STEP:CRH?	
Parameter	<NRf>[mS] MINIMUM or MIN MAXIMUM or MAX	Step resolution (Unit: mS) Minimum step resolution Maximum step resolution

Return parameter	<ASCII string>	Returns the range and the step resolution.
------------------	----------------	--

Example	:STEP:CRH 0.8 Sets the step resolution to 0.8 mS.
---------	--

Query example	:STEP:CRH? >CRH:0.8 Returns the step resolution (0.8 mS).
---------------	---

[[:CONFigure]:STEP:CRM

Set →

→ Query

Description	Configures the step resolution for CR Medium Range. Note: The step resolution setting will be automatically rounded to the closest multiple of the base resolution.
-------------	---

Syntax	[[:CONFigure]:STEP:CRM {<NRf>[mS] MINimum MAXimum }
--------	---

Query Syntax	[[:CONFigure]:STEP:CRM?
--------------	-------------------------

Parameter	<NRf>[mS] MINIMUM or MIN MAXIMUM or MAX	Step resolution (Unit: mS) Minimum step resolution Maximum step resolution
-----------	---	--

Return parameter	<ASCII string>	Returns the range and the step resolution.
------------------	----------------	--

Example	:STEP:CRM 0.08 Sets the step resolution to 0.08 mS.
---------	--


Query example	:STEP:CRM? >CRM:0.08 Returns the step resolution (0.08 mS).
---------------	---


[[:CONFigure]:STEP:CRL (Set) →
→ (Query)

Description	Configures the step resolution for CR Low Range. Note: The step resolution setting will be automatically rounded to the closest multiple of the base resolution.	
Syntax	[:CONFigure]:STEP:CRL {<NRf>[mS] MINimum MAXimum }	
Query Syntax	[:CONFigure]:STEP:CRL?	
Parameter	<NRf>[mS] MINIMUM or MIN MAXIMUM or MAX	Step resolution (Unit: mS) Minimum step resolution Maximum step resolution
Return parameter	<ASCII string>	Returns the range and the step resolution.
Example	:STEP:CRL 0.008 Sets the step resolution to 0.008 mS.	
Query example	:STEP:CRL? >CRL:0.008 Returns the step resolution (0.008 mS).	

[[:CONFigure]:STEP:CR → (Query)


Description	Returns the step resolution for each CR Mode range as a string.	
Query Syntax	[:CONFigure]:STEP:CR?	
Return parameter	<ASCII string>	Returns the CRH, CRM and CRL step resolution settings (in mS).
Query example	:STEP:CR? > CRH:0.8, CRM:0.08, CRL:0.008 Returns the CR mode step resolution for each range (mS).	






[[:CONFigure]:STEP:CVH

Description	Configures the step resolution for CV High Range. Note: The step resolution setting will be automatically rounded to the closest multiple of the base resolution.	
Syntax	[:CONFigure]:STEP:CVH{<NRf>[V] MINimum MAXimum}	
Query Syntax	[:CONFigure]:STEP:CVH?	
Parameter	<NRf>[V] MINIMUM or MIN MAXIMUM or MAX	Step resolution. Minimum step resolution Maximum step resolution
Return parameter	<ASCII string>	Returns the range and the step resolution.
Example	:STEP:CVH 0.01V Sets the step resolution to 0.01V.	
Query example	:STEP:CVH? > CVH:0.01 Returns the step resolution (0.01V).	





[[:CONFigure]:STEP:CVL

Description	Configures the step resolution for CV Low Range. Note: The step resolution setting will be automatically rounded to the closest multiple of the base resolution.	
Syntax	[:CONFigure]:STEP:CVL{<NRf>[V] MINimum MAXimum}	
Query Syntax	[:CONFigure]:STEP:CVL?	
Parameter	<NRf>[V] MINIMUM or MIN MAXIMUM or MAX	Step resolution. Minimum step resolution Maximum step resolution
Return parameter	<ASCII string>	Returns the range and the step resolution.

Example :STEP:CVL 0.001V
Sets the step resolution to 0.001V.

Query example :STEP:CVL?
> CVH:0.001
Returns the step resolution (0.001V).

[:CONFigure]:STEP:CV → Query

Description Returns the step resolution for each CV Mode range as a string.

Query Syntax [:CONFigure]:STEP:CV?

Return parameter <ASCII string> Returns the CVH and CVL step resolution settings.

Query example :STEP:CV?
>CVH:0.01, CVL:0.001
Returns the CV mode step resolution for each range.

Set →

[:CONFigure]:STEP:CPH → Query

Description Configures the step resolution for CP High Range. Note: The step resolution setting will be automatically rounded to the closest multiple of the base resolution.

Syntax [:CONFigure]:STEP:CPH {<NRf>[W] | MINimum | MAXimum }

Query Syntax [:CONFigure]:STEP:CPH?

Parameter <NRf>[W] Step resolution.
MINIMUM or MIN Minimum step resolution
MAXIMUM or MAX Maximum step resolution

Return parameter <ASCII string> Returns the range and the step resolution.

Example :STEP:CPH 0.01
Sets the step resolution to 0.01W.

Query example :STEP:CPH?
>CPH:0.01
Returns the step resolution (0.01W).

Set →

→ Query

[[:CONFIgure]:STEP:CPM

Description Configures the step resolution for CP Medium Range. Note: The step resolution setting will be automatically rounded to the closest multiple of the base resolution.

Syntax [[:CONFIgure]:STEP:CPM {<NRF>[W] | MINimum | MAXimum }

Query Syntax [[:CONFIgure]:STEP:CPM?

Parameter	<NRF>[W]	Step resolution.
	MINIMUM or MIN	Minimum step resolution
	MAXIMUM or MAX	Maximum step resolution

Return parameter	<ASCII string>	Returns the range and the step resolution.
-------------------------	----------------	--

Example :STEP:CPM 0.001
Sets the step resolution to 0.001W.

Query example :STEP:CPM?
>CPM:0.001
Returns the step resolution (0.001W).

Set →

→ Query

[[:CONFIgure]:STEP:CPL

Description Configures the step resolution for CP Low Range. Note: The step resolution setting will be automatically rounded to the closest multiple of the base resolution.

Syntax [[:CONFIgure]:STEP:CPL {<NRF>[W] | MINimum | MAXimum }

Query Syntax [[:CONFIgure]:STEP:CPL?

Parameter	<NRF>[W]	Step resolution.
	MINIMUM or MIN	Minimum step resolution

	MAXIMUM or MAX	Maximum step resolution
Return parameter	<ASCII string>	Returns the range and the step resolution.
Example	:STEP:CPL 0.0001 Sets the step resolution to 0.0001W.	
Query example	:STEP:CPL? >CPM:0.0001 Returns the step resolution (0.0001W).	

[[:CONFigure]:STEP:CP → Query

Description	Returns the step resolution for each CP Mode range as a string.	
Query Syntax	[:CONFigure]:STEP:CP?	
Return parameter	<ASCII string>	Returns the CPH, CPM and CPL step resolution settings.
Query example	:STEP:CP? > CPH:0.01, CPM:0.001, CPL:0.0001 Returns the CP mode step resolution for each range.	

External Control Commands

[:CONFigure]:EXTernal[:CONTrol]	65
[:CONFigure]:EXTernal:LOADonin	65

[:CONFigure]:EXTernal[:CONTrol]




Description Configures the unit for external control or disables external control.

Syntax [:CONFigure]:EXTernal[:CONTrol] {OFF | VOLTage | RESistance | RINV }

Related Commands [:CONFigure]:EXTernal[:CONTrol]?

Parameter	OFF	Disables external control
	VOLTAGE or VOLT	Sets the unit to external voltage control
	RESISTANCE or RES	Sets the unit to external resistance control
	RINV	Sets the unit to external resistance (inverted) control

Return Parameter <ASCII string> Returns the external control configuration

Example :EXTernal VOLT
Turns external control voltage control on.

Query example :EXTernal?
>voltage
The unit uses external voltage control.

[:CONFigure]:EXTernal:LOADonin




Description The LOADonin settings determine whether the load is turned on when an external switch is closed (LOW) or open (HIGH).

Syntax	[:CONFigure]:EXTernal:LOADonin {OFF HIGH LOW }	
Related Commands	[:CONFigure]:EXTernal:LOADonin?	
Parameter	OFF HIGH LOW	LoadOnIN = OFF LoadOnIN = OPEN LoadOnIN = CLOSE
Return Parameter	<ASCII string>	Returns the Loadonin configuration as a string.
Example	:EXTernal:LOADonin OFF Turns external control off.	
Query example	:EXTernal:LOADonin? > OFF External control is off	

Mode Subsystem Commands

:MODE.....	67
[:MODE]:CRANge.....	67
[:MODE]:VRANge.....	68
[:MODE]:RESPonse.....	68
[:MODE]:DYNamic.....	69

:MODE




Description	Sets the operating mode.	
Syntax	:MODE {CC CR CV CP CCCV CRCV CPCV }	
Query Syntax	:MODE?	
Parameter/Return parameter	CC	CC mode
	CR	CR mode
	CV	CV mode
	CP	CP mode
	CCCV	CC + CV mode
	CRCV	CR + CV mode
	CPCV	CP + CV mode
Example	:MODE CC Sets the mode to CC mode.	
Query example	:MODE? >CC Returns the operating mode (CC mode).	

[:MODE]:CRANge




Description	Configures the current range for all the applicable operating modes.	
Syntax	[:MODE]:CRANge {HIGH MIDDLE LOW }	
Query Syntax	[:MODE]:CRANge?	

Parameter	HIGH MIDDLE or MIDD LOW	High range Middle range Low range
Return parameter	High Mid Low	High range Middle range Low range

Example :CRANge LOW
Sets the current range to Low.

Query example :CRANge?
>Low
The current range is set to Low.

Set →

→ Query

[:MODE] :VRANge

Description Configures the voltage range for all the applicable operating modes.

Syntax [:MODE] :VRANge { HIGH | LOW }

Query Syntax [:MODE] :VRANge?

Parameter	HIGH LOW	High range Low range
-----------	-------------	-------------------------

Return parameter	High Low	High range Low range
------------------	-------------	-------------------------

Example :VRANge LOW
Sets the voltage range to Low.

Query example :VRANge?
>LOW
The voltage range is set to Low.

Set →

→ Query

[:MODE] :RESPonse

Description Returns the CV Mode response speed. Fast is the default response speed.

Syntax [:MODE] :RESPonse { FAST | SLOW }

Query Syntax [:MODE] :RESPonse?

Parameter	FAST	Fast response
	SLOW	Slow response
Return parameter	<ASCII string>	Returns CV response speed as a string.
Example	:RESPonse FAST Sets the CV response to fast.	
Query example	:RESPonse? > CV mode response:FAST.	


[:MODE]:DYNamic


Description	Sets or queries the switching mode. Dynamic is the default mode.	
Syntax	:MODE:DYNamic{ DYNamic STATic }	
Query Syntax	:MODE:DYNamic?	
Parameter	DYNAMIC or DYN STATIC or STAT	Set to Dynamic mode Set to Static mode
Return parameter	<ASCII string>	Returns the switching mode.
Example	:MODE:DYNamic DYN? Set the switching mode to dynamic	
Query example	:MODE:DYNamic? > Dynamic, ;Dynamic Level:Value, Dynamic Time:T1/T2 The switching mode is set to dynamic mode.	

Current Subsystem Commands

:CURRent[:VA].....	70
:CURRent:VB	71
:CURRent:SRATe	71
:CURRent:L1.....	72
:CURRent:L2.....	72
:CURRent:SET	73
:CURRent:LEVel.....	74
:CURRent:RISE.....	74
:CURRent:FALL	75
:CURRent:T1	75
:CURRent:T2	76
:CURRent:FREQuency.....	77
:CURRent:DUTY.....	77

:CURRent[:VA]



Description Sets or queries the CC mode “A Value” (static mode) current. This command is applicable to static modes.

Note: A different current value can be set for each current range (High/Mid/Low).

Note: The [:VA] node can only be omitted when in static mode.

Syntax :CURRent[:VA] {<NRf>[A] | MINimum | MAXimum }

Query Syntax :CURRent[:VA]?

Parameter	<NRf>[A] MINIMUM or MIN MAXIMUM or MAX	“A Value” current value Minimum current level Maximum current level
------------------	--	---

Return parameter	<NR2>	Returns the “A Value” current value.
-------------------------	-------	--------------------------------------

Example :CURRent:VA MIN
Sets the current value to the minimum.

Query example :CURRent:VA?
>1.0A

Returns the “A Value” current setting.

Set →

→ Query

:CURRent:VB

Description Sets or queries the CC mode “B Value” (static mode) current. This command is applicable to static modes.

Note: A different current value can be set for each current range (High/Mid/Low).

Syntax :CURRent:VB {<NRf>[A] | MINimum | MAXimum }

Query Syntax :CURRent:VB?

Parameter	<NRf>[A] MINIMUM or MIN MAXIMUM or MAX	“B Value” current value Minimum current level Maximum current level
------------------	--	---

Return parameter	<NR2>	Returns the “B Value” current value.
-------------------------	-------	--------------------------------------

Example :CURRent:VB MIN
Sets the current value to the minimum.

Query example :CURRent:VB?
>1.0A
Returns the “B Value” current setting.

Set →

→ Query

:CURRent:SRATe

Description Sets or queries the current slew rate for CC static mode.

Syntax :CURRent:SRATe {<NRf>| MINimum | MAXimum }

Query Syntax :CURRent:SRATe?

Parameter	<NRf> MINIMUM or MIN MAXIMUM or MAX	Sets the slew rate in mA/us Set to the highest slew rate Set to the lowest slew rate
------------------	---	--

Return parameter	<code><NR2></code>	Returns the slew rate in mA/us.
------------------	--------------------------	---------------------------------

Example	<pre>:CURRent:SRATe MIN</pre> <p>Sets the slew rate to the minimum.</p>
---------	---

Query example	<pre>:CURRent:SRATe? >5.0</pre> <p>Returns the slew rate as 5.0mA/us.</p>
---------------	--

(Set) →

← (Query)

`:CURRent:L1`

Description	<p>Sets or queries the CC mode “Level 1” current. This command is only applicable to dynamic modes.</p> <p>Note: A different current value can be set for each range (High/Mid/Low).</p>
-------------	--

Syntax	<code>:CURRent:L1 {<NRf>[A] MINimum MAXimum }</code>
--------	--

Query Syntax	<code>:CURRent:L1?</code>
--------------	---------------------------

Parameter	<pre><NRf>[A] MINIMUM or MIN MAXIMUM or MAX</pre>	<p>“Level1” current value</p> <p>Minimum current level</p> <p>Maximum current level</p>
-----------	---	---

Return parameter	<code><NR2></code>	Returns the “Level1” current value.
------------------	--------------------------	-------------------------------------

Example	<pre>:CURRent:L1 MIN</pre> <p>Sets the current value to the minimum.</p>
---------	--

Query example	<pre>:CURRent:L1? >1.0A</pre> <p>Returns the “Level1” current setting.</p>
---------------	---

(Set) →

← (Query)

`:CURRent:L2`

Description	<p>Sets or queries the CC mode “Level2” current. This command is only applicable to dynamic modes.</p> <p>Note: A different current value can be set for each range (High/Mid/Low).</p>
-------------	---

Syntax :CURRent:L2 {<NRf>[A] | MINimum | MAXimum }


Query Syntax :CURRent:L2?

Parameter	<NRf>[A] MINIMUM or MIN MAXIMUM or MAX	“Level2” current value Minimum current level Maximum current level
-----------	--	--

Return parameter	<NR2>	Returns the “Level2” current value.
------------------	-------	-------------------------------------

Example :CURRent:L2 MIN
Sets the current value to the minimum.

Query example :CURRent:L2?
>1.0A
Returns the “Level2” current setting.



:CURRent:SET

Description Sets or queries the CC dynamic mode Set value when the dynamic units are set to Percent.
This command is only applicable in dynamic mode.

Syntax :CURRent:SET{<NRf>[A] | MINimum | MAXimum }

Query Syntax :CURRent:SET?

Related Commands :CURRent:LEVel

Parameter	<NRf>[A] MINIMUM or MIN MAXIMUM or MAX	“Set” current value Minimum current level Maximum current level
-----------	--	---

Return parameter	<NR2>	Returns the “Set” current value.
------------------	-------	----------------------------------

Example :CURRent:SET MIN
Sets the current value to the minimum.

Query example :CURRent:SET?
>1.0A
Returns the “Set” current setting.

:CURRent:LEVel

Set →

→ Query

Description	Sets or queries the CC mode % level (percentage of the Set current value) when the dynamic mode units are set to Percent.	
Syntax	:CURRent:LEVel {<NRf> MINimum MAXimum }	
Query Syntax	:CURRent:LEVel?	
Related Commands	:CURRent:SET	
Parameter	<NRf> MINIMUM or MIN MAXIMUM or MAX	“% level” current value Minimum % current level Maximum % current level
Return parameter	<NR2>	Returns the “% level” current value.
Example	:CURRent:LEVel MIN Sets the % level current value to the minimum.	
Query example	:CURRent:LEVel? >50 Returns the “% Level” as 50 percent.	

Set →


→ Query

:CURRent:RISE

Description	Sets the rising current slew rate for CC dynamic mode.	
Syntax	:CURRent:RISE {<NRf> MINimum MAXimum }	
Query Syntax	:CURRent:RISE?	
Related Commands	:CURRent:FALL	
Parameter	<NRf> MINIMUM or MIN MAXIMUM or MAX	Rising current slew rate Minimum slew rate Maximum slew rate
Return parameter	<NR2>	Returns the rising current slew rate in mA/us.

Example :CURRent:RISE MIN
Sets the rising slew rate to the minimum.

Query example :CURRent:RISE?
>5000
Returns the rising slew rate as 5000mA/us.



:CURRent:FALL

Description Sets the falling current slew rate for CC dynamic mode.

Syntax :CURRent:FALL {<NRf> | MINimum | MAXimum }

Query Syntax :CURRent:FALL?


Related Commands :CURRent:FALL

Parameter	<NRf> MINIMUM or MIN MAXIMUM or MAX	Falling current slew rate Minimum slew rate Maximum slew rate
-----------	---	---

Return parameter	<NR2>	Returns the falling current slew rate in mA/us.
------------------	-------	---

Example :CURRent:FALL MIN
Sets the falling slew rate to the minimum.

Query example :CURRent:FALL?
>5000
Returns the falling slew rate as 5000mA/us.



:CURRent:T1

Description Sets the T1 timer settings for the CC dynamic mode.

Syntax :CURRent:T1 {<NRf>[s] | MINimum | MAXimum}


Query Syntax :CURRent:T1?

Related Commands :CURRent:T2

Parameter	<NRf>[s] MINIMUM or MIN MAXIMUM or MAX	T1 timer setting in seconds Minimum time Maximum time
Return parameter	<NR2>	Returns the T1 timer time in seconds.

Example :CURRent:T1 0.200
Sets the T1 timer time to 200ms.

Query example :CURRent:T1?
>0.200
Returns the T1 timer time as 200ms.



:CURRent:T2

Description	Sets the T2 timer settings for the CC dynamic mode.	
Syntax	:CURRent:T2 {<NRf>[s] MINimum MAXimum}	
Query Syntax	:CURRent:T2?	
Related Commands	:CURRent:T1	

Parameter	<NRf>[s] MINIMUM or MIN MAXIMUM or MAX	T2 timer setting in seconds Minimum time Maximum time
Return parameter	<NR2>	Returns the T2 timer time in seconds.

Example :CURRent:T2 0.200
Sets the T2 timer time to 200ms.

Query example :CURRent:T2?
>0.200
Returns the T2 timer time as 200ms.

:CURRent:FREQuency



Description Sets the CC dynamic mode switching frequency. This command along with the “:CURRent:DUTY” command is used when the dynamic time setting is set to “Freq./Duty”.

This command is only applicable for dynamic mode.

Syntax :CURRent:FREQuency {<NRF> | MINIMUM | MAXIMUM}

Query Syntax :CURRent:FREQuency?

Related Commands :CURRent:DUTY

Parameter	<NRF>	Sets the switching frequency in hertz.
	MINIMUM or MIN	Minimum frequency
	MAXIMUM or MAX	Maximum frequency

Return parameter <NR2> Returns the frequency in hertz

Example :CURRent:FREQuency 60
Sets frequency to 60Hz.

Query example :CURRent:FREQuency?
>60
Returns the switching frequency (60Hz).

:CURRent:DUTY



Description Sets the positive duty cycle for the CC dynamic mode switching frequency. This command along with the “:CURRent:FREQuency” command is used when the dynamic time setting is set to “Freq./Duty”.

This command is only applicable for dynamic mode.

Syntax	:CURRent:DUTY {<NRf> MINimum MAXimum}	
Query Syntax	:CURRent:DUTY?	
Related Commands	:CURRent:FREQuency	
Parameter	<NRf> MINIMUM or MIN MAXIMUM or MAX	Sets the duty as a percentage. Minimum duty Maximum duty
Return parameter	<NR2>	Returns the duty as a percentage
Example	:CURRent:DUTY 50 Sets the duty to 50%.	
Query example	:CURRent:DUTY? >50 Returns the duty (50%).	

Resistance Subsystem Commands

- :CONDuctance[:VA].....
- :CONDuctance:VB.....
- :RESistance[:VA].....
- :RESistance:VB.....
- :RESistance:SRATe.....
- :CONDuctance:L1.....
- :CONDuctance:L2.....
- :CONDuctance:SET
- :RESistance:L1.....
- :RESistance:L2.....
- :RESistance:SET
- :RESistance:LEVel.....
- :RESistance:RISE.....
- :RESistance:FALL
- :RESistance:T1.....
- :RESistance:T2.....
- :RESistance:FREQuency.....
- :RESistance:DUTY.....
- Voltage Subsystem Commands
- :VOLTage[:VA].....
- :VOLTage:VB.....


:CONDuctance[:VA]


Description	<p>Sets or queries the CR mode “A Value” conductance. This command is only applicable to static mode.</p> <p>Note: A different value can be set for each current range (High/Mid/Low).</p> <hr/> <p>Note: The optional command node [:VA] can only be omitted when in static mode.</p>
Syntax	:CONDuctance[:VA] {<NRf>[mS] MINimum MAXimum }
Query Syntax	:CONDuctance[:VA]?

Parameter	<NRf>[mS] MINIMUM or MIN MAXIMUM or MAX	“A Value” conductance value (Unit: millisiemens) Minimum conductance level Maximum conductance level
Return parameter	<NR2>	Returns the “A Value” conductance value

Example :CONDuctance:VA MIN
Sets the conductance value to the minimum.

Query example :CONDuctance:VA?
> 0
Returns the “A Value” conductance setting(mS).



:CONDuctance:VB

Description Sets or queries the CR mode “B Value” conductance. This command is applicable to static mode only.
Note: A different value can be set for each current range (High/Mid/Low).

Syntax :CONDuctance:VB {<NRf>[mS] | MINimum | MAXimum }

Query Syntax :CONDuctance:VB?

Parameter	<NRf>[mS] MINIMUM or MIN MAXIMUM or MAX	“B Value” conductance value Minimum conductance level Maximum conductance level
Return parameter	<NR2>	Returns the “B Value” conductance value

Example :CONDuctance:VB MIN
Sets the conductance value to the minimum.

Query example :CONDuctance:VB?
> 0
Returns the “B Value” conductance setting(mS).

Set →

→ Query

:RESistance[:VA]

Description Sets or queries the CR mode “A Value” resistance. This command is only applicable to static mode.
Note: A different value can be set for each current range (High/Mid/Low).
Note: The optional command node [:VA] can only be omitted when in static mode.

Syntax :RESistance[:VA] {<NRF>[OHM] | MINimum | MAXimum }

Query Syntax :RESistance[:VA]?

Parameter	<NRF>[OHM] MINIMUM or MIN MAXIMUM or MAX	“A Value” resistance value Minimum resistance level Maximum resistance level
-----------	--	--

Return parameter	<NR2>	Returns the “A Value” resistance value
------------------	-------	--

Example :RESistance:VA MIN
Sets the resistance value to the minimum.

Query example :RESistance:VA?
> 0.04082
Returns the “A Value” resistance setting(OHM).

Set →

→ Query

:RESistance:VB


Description Sets or queries the CR mode “B Value” resistance. This command is applicable to static mode only.
Note: A different value can be set for each current range (High/Mid/Low).

Syntax :RESistance:VB {<NRF>[OHM] | MINimum | MAXimum }

Query Syntax	:RESistance:VB?	
Parameter	<NRf>[OHM] MINIMUM or MIN MAXIMUM or MAX	“B Value” resistance value Minimum resistance level Maximum resistance level
Return parameter	<NR2>	Returns the “B Value” resistance value

Example :RESistance:VB MIN
Sets the resistance value to the minimum.

Query example :RESistance:VB?
> 0.04082
Returns the “B Value” resistance setting(OHM).



:RESistance:SRATe

Description Sets or queries the current slew rate for CR static mode.

Syntax :RESistance:SRATe {<NRf> | MINimum | MAXimum}


Query Syntax :RESistance:SRATe?

Parameter	<NRf> MINIMUM or MIN MAXIMUM or MAX	Sets the slew rate in mA/us Set to the lowest slew rate Set to the highest slew rate
-----------	---	--

Return parameter <NR2>
Returns the slew rate in mA/us

Example :RESistance:SRATe MIN
Sets the slew rate to the minimum.

Query example :RESistance:SRATe?
>5.0000
Returns the slew rate as 5mA/us.



:CONDuctance:L1

Description Sets or queries the CR mode “Level1” conductance. This command is only applicable to dynamic mode.
 Note: A different value can be set for each current range (High/Mid/Low).

Syntax :CONDuctance:L1 {<NRF>[mS] | MINimum | MAXimum }


Query Syntax :CONDuctance:L1?

Parameter	<NRF>[mS]	“level1” conductance value (Unit: millisiemens)
	MINIMUM or MIN	Minimum conductance level
	MAXIMUM or MAX	Maximum conductance level

Return parameter <NR2> Returns the “level1” conductance value

Example :CONDuctance:L1 MIN
 Sets the conductance value to the minimum.

Query example :CONDuctance:L1?
 > 0
 Returns the “level1” conductance setting(mS).



:CONDuctance:L2

Description Sets or queries the CR mode “level2” conductance. This command is applicable to dynamic mode only.
 Note: A different value can be set for each current range (High/Mid/Low).


Syntax :CONDuctance:L2 {<NRF>[mS] | MINimum | MAXimum }

Query Syntax :CONDuctance:L2?

Parameter	<NRf> MINIMUM or MIN MAXIMUM or MAX	“level2” conductance value (Unit: millisiemens) Minimum conductance level Maximum conductance level
Return parameter	<NR2>	Returns the “Level2” conductance value

Example :CONDuctance:L2 MIN
Sets the conductance value to the minimum.

Query example :CONDuctance:L2?
> 0
Returns the “Level2” conductance setting(mS).



:CONDuctance:SET

Description Sets or queries the CR dynamic mode Set value when the dynamic units are set to Percent.
This command is only applicable in dynamic mode.

Syntax :CONDuctance:SET {<NRf>[mS] | MINimum | MAXimum }


Query Syntax :CONDuctance:SET?

Related Commands :CONDuctance:LEVel

Parameter	<NRf> MINIMUM or MIN MAXIMUM or MAX	“Set” conductance value (Unit: mS) Minimum conductance level Maximum conductance level
Return parameter	<NR2>	Returns the “Set” conductance value (Unit: mS)

Example :CONDuctance:SET MIN
Sets the conductance to the minimum.

Query example :CONDuctance:SET?
> 0
Returns the “Set” conductance setting in mS.



:RESistance:L1

Description Sets or queries the CR mode “Level1” resistance. This command is only applicable to dynamic mode.
Note: A different value can be set for each current range (High/Mid/Low).

Syntax :RESistance:L1 {<NRF>[OHM] | MINimum | MAXimum }

Query Syntax :RESistance:L1?

Parameter	<NRF>[OHM]	“level1” resistance value (Unit: OHM)
	MINIMUM or MIN	Minimum resistance level
	MAXIMUM or MAX	Maximum resistance level

Return parameter <NR2>
Returns the “level1” resistance value

Example :RESistance:L1 MIN
Sets the resistance value to the minimum.

Query example :RESistance:L1?
> 0.04082
Returns the “level1” resistance setting(OHM).

Set →

→ Query

:RESistance:L2

Description Sets or queries the CR mode “level2” resistance. This command is applicable to dynamic mode only.
 Note: A different value can be set for each current range (High/Mid/Low).

Syntax :RESistance:L2 {<NRf>[OHM] | MINimum | MAXimum }

Query Syntax :RESistance:L2?

Parameter	<NRf> MINIMUM or MIN MAXIMUM or MAX	“level2” resistance value Minimum resistance level Maximum resistance level
------------------	---	---

Return parameter	<NR2>	Returns the “level2” resistance value
-------------------------	-------	---------------------------------------

Example :RESistance:L2 MIN
 Sets the resistance value to the minimum.

Query example :RESistance:L2?
 > 0.04082
 Returns the “level2” resistance setting.(OHM)

Set →

→ Query

:RESistance:SET

Description Sets or queries the CR dynamic mode Set value when the dynamic units are set to Percent. This command is only applicable in dynamic mode.

Syntax :RESistance:SET {<NRf>[OHM] | MINimum | MAXimum }


Query Syntax :RESistance:SET?

Related Commands :RESistance:LEVel

Parameter	<NRf>	“Set” resistance value (Unit: OHM)
	MINIMUM or MIN	Minimum resistance level
	MAXIMUM or MAX	Maximum resistance level
Return parameter	<NR2>	Returns the “Set” resistance value.

Example :RESistance:SET MIN
Sets the resistance to the minimum.

Query example :RESistance:SET?
 > 0.04082
Returns the “Set” resistance setting in OHM.



:RESistance:LEVel

Description Sets or queries the CR mode % level (percentage of the Set conductance value) when the dynamic mode units are set to Percent.

Syntax :RESistance:LEVel {<NRf> | MINimum | MAXimum }

Query Syntax :RESistance:LEVel?

Related Commands :RESistance:SET

Parameter	<NRf>	“% level” conductance value
	MINIMUM or MIN	Minimum % conductance level
	MAXIMUM or MAX	Maximum % conductance level

Return parameter <NR2> Returns the “% level” conductance value.

Example :RESistance:LEVel MIN
Sets the % level conductance value to the minimum.

Query example :RESistance:LEVel?
 >50
Returns the “% Level” as 50 percent.

Set →

→ Query

:RESistance:RISE

Description	Sets the rising current slew rate for CR dynamic mode.	
Syntax	:RESistance:RISE {<NRf> MINimum MAXimum }	
Query Syntax	:RESistance:RISE?	
Related Commands	:RESistance:FALL	
Parameter	<NRf> MINIMUM or MIN MAXIMUM or MAX	Rising current slew rate [mA/us] Minimum slew rate Maximum slew rate
Return parameter	<NR2>	Returns the rising current slew rate in mA/us.
Example	:RESistance:RISE MIN Sets the rising slew rate to the minimum.	
Query example	:RESistance:RISE? >50.000 Returns the rising slew rate as 50mA/us.	

Set →


→ Query

:RESistance:FALL

Description	Sets the falling current slew rate for CR dynamic mode.	
Syntax	:RESistance:FALL {<NRf> MINimum MAXimum }	
Query Syntax	:RESistance:FALL?	
Related Commands	:RESistance:RISE	
Parameter	<NRf> MINIMUM or MIN MAXIMUM or MAX	Falling current slew rate [mA/us] Minimum slew rate Maximum slew rate
Return parameter	<NR2>	Returns the falling current slew rate in mA/us.

Example	:RESistance:FALL MIN Sets the falling slew rate to the minimum.
Query example	:RESistance:FALL? >50.000 Returns the falling slew rate as 50mA/us.

:RESistance:T1




Description	Sets the T1 timer settings for the CR dynamic mode.	
Syntax	:RESistance:T1 {<NRf>[s] MINimum MAXimum}	
Query Syntax	:RESistance:T1?	
Related Commands	:RESistance:T2	
Parameter	<NRf>[s] MINIMUM or MIN MAXIMUM or MAX	T1 timer setting in seconds Minimum time Maximum time
Return parameter	<NR2>	Returns the T1 timer time in seconds.

Example	:CURRent:T1 0.200 :CURRent:T1 0.200s :CURRent:T1 200 ms Sets the T1 timer time to 200ms.
---------	---

Query example	:CURRent:T1? >0.200 Returns the T1 timer time as 200ms.
---------------	---

:RESistance:T2



Description	Sets the T2 timer settings for the CR dynamic mode.	
Syntax	:RESistance:T2 {<NRf>[s] MINimum MAXimum}	

Query Syntax	:RESistance:T2?	
Related Commands	:RESistance:T1	
Parameter	<NRf>[s] MINIMUM or MIN MAXIMUM or MAX	T2 timer setting in seconds Minimum time Maximum time
Return parameter	<NR2>	Returns the T2 timer time in seconds.
Example	:RESistance:T2 0.200 Sets the T2 timer time to 200ms.	
Query example	:RESistance:T2? >0.200 Returns the T2 timer time as 200ms.	

Set →

← Query


:RESistance:FREQUENCY

Description	Sets the CR dynamic mode switching frequency. This command along with the “:RESistance:DUTY” command is used when the dynamic time setting is set to “Freq./Duty”. This command is only applicable for dynamic mode.	
Syntax	:RESistance:FREQUENCY {<NRf> MINimum MAXimum}	
Query Syntax	:RESistance:FREQUENCY?	
Related Commands	:RESistance:DUTY	
Parameter	<NRf> MINIMUM or MIN MAXIMUM or MAX	Sets the switching frequency in hertz. Minimum frequency Maximum frequency
Return parameter	<NR2>	Returns the frequency in hertz.

Example :RESistance:FREQuency 60
Sets frequency to 60Hz.

Query example :RESistance:FREQuency?
>60
Returns the switching frequency (60Hz).

:RESistance:DUTY



Description Sets the positive duty cycle for the CR dynamic mode switching frequency. This command along with the “:RESistance:FREQuency” command is used when the dynamic time setting is set to “Freq./Duty”.
This command is only applicable for dynamic mode.

Syntax :RESistance:DUTY {<NRf> | MINimum | MAXimum}

Query Syntax :RESistance:DUTY?

Related Commands :RESistance:FREQuency

Parameter	<NRf> MINIMUM or MIN MAXIMUM or MAX	Sets the duty as a percentage. Minimum duty Maximum duty
Return parameter	<NR2>	Returns the duty as a percentage.

Example :RESistance:DUTY 50
Sets the duty to 50%.

Query example :RESistance:DUTY?
>50
Returns the duty (50%).

Voltage Subsystem Commands

:VOLTage[:VA]	92
:VOLTage:VB	92

:VOLTage[:VA]

Description Sets or queries the CV mode “A Value” voltage or the +CV voltage value. Note: The same value applies for each current range (High/Mid/Low).

Note: The optional command node [:VA] can only be omitted when in static mode.

Syntax :VOLTage[:VA] {<NRf>[V] | MINimum | MAXimum }

Query Syntax :VOLTage[:VA]?

Parameter	<NRf>[V]	“A Value” voltage value
	MINIMUM or MIN	Minimum voltage level
	MAXIMUM or MAX	Maximum voltage level

Return parameter	<NR2>	Returns the “A Value” voltage value.
-------------------------	-------	--------------------------------------

Example :VOLTage:VA MIN

 Sets the voltage value to the minimum.

Query example :VOLTage:VA?

 >1.000V

 Returns the “A Value” voltage setting.

:VOLTage:VB

Description Sets or queries the CV mode “B Value”. Note: The same value applies for each current range (High/Mid/Low).

Syntax :VOLTage:VB {<NRf>[V] | MINimum | MAXimum }


Query Syntax :VOLTage:VB?

Parameter	<NRf>[V] MINIMUM or MIN MAXIMUM or MAX	“B Value” voltage value Minimum voltage level Maximum voltage level
Return parameter	<NR2>	Returns the “B Value” voltage value.
Example	:VOLTage:VB MIN Sets the voltage value to the minimum.	
Query example	:VOLTage:VB? >1.000V Returns the “B Value” voltage setting.	


Power Subsystem Commands


:POWer[:VA].....	94
:POWer:VB	95
:POWer:L1	95
:POWer:L2	96
:POWer:SET	96
:POWer:LEVel	97
:POWer:T1	98
:POWer:T2	98
:POWer:FREQuency.....	99
:POWer:DUTY.....	100

:POWer[:VA]




Description	Sets or queries the CP mode “A Value” power. This command is applicable to static mode only. Note: A different “A Value” can be set for different current ranges. Note: The [:VA] node can only be omitted when in static mode.	
Syntax	:POWer[:VA] {<NRf>[W] MINimum MAXimum }	
Query Syntax	:POWer[:VA]?	
Parameter	<NRf>[W] MINIMUM or MIN MAXIMUM or MAX	“A Value” power value Minimum power level Maximum power level
Return parameter	<NR2>	Returns the “A Value” power value.
Example	:POWer:VA MIN Sets the power value to the minimum.	
Query example	:POWer:VA? >10W Returns the “A Value” power setting.	






:POWer:VB

Description	Sets or queries the CP mode “B Value” power. This command is only applicable to static mode. Note: A different “B Value” can be set to different current ranges.	
Syntax	:POWer:VB {<NRf>[W] MINimum MAXimum }	
Query Syntax	:POWer:VB?	
Parameter	<NRf>[W] MINIMUM or MIN MAXIMUM or MAX	“B Value” power value Minimum power level Maximum power level
Return parameter	<NR2>	Returns the “B Value” power value.
Example	:POWer:VB MIN Sets the power value to the minimum.	
Query example	:POWer:VB? >10W Returns the “B Value” power setting.	






:POWer:L1

Description	Sets or queries the CP mode “Level1” power. This command is applicable to dynamic mode only. Note: A different “Level1” value can be set for different current ranges.	
Syntax	:POWer:L1 {<NRf>[W] MINimum MAXimum }	
Query Syntax	:POWer:L1?	
Parameter	<NRf>[W] MINIMUM or MIN MAXIMUM or MAX	“Level1” power value Minimum power level Maximum power level
Return parameter	<NR2>	Returns the “Level1” power value.

Example :POWer:L1 MIN
Sets the power value to the minimum.

Query example :POWer:L1?
>10W
Returns the “Level1” power setting.

:POWer:L2



Description Sets or queries the CP mode “Level2” power. This command is only applicable to dynamic mode.
Note: A different “Level2” value can be set to different current ranges.

Syntax :POWer:L2 {<NRf>[W] | MINimum | MAXimum }

Query Syntax :POWer:L2?


Parameter	<NRf>[W]	“Level2” power value
	MINIMUM or MIN	Minimum power level
	MAXIMUM or MAX	Maximum power level

Return parameter	<NR2>	Returns the “Level2” power value.
------------------	-------	-----------------------------------

Example :POWer:L2 MIN
Sets the power value to the minimum.

Query example :POWer:L2?
>10W
Returns the “Level2” power setting.

:POWer:SET




Description Sets or queries the CP dynamic mode Set value when the dynamic units are set to Percent.
This command is only applicable in dynamic mode.

Syntax :POWer:SET {<NRf>[W] | MINimum | MAXimum }

Query Syntax :POWer:SET?

Related Commands	:POWer:LEVel	
Parameter	<NRf>[W] MINIMUM or MIN MAXIMUM or MAX	“Set” power value Minimum power level Maximum power level
Return parameter	<NR2>	Returns the “Set” power value.
Example	:POWer:SET MIN Sets the power value to the minimum.	
Query example	:POWer:SET? >10W Returns the “Set” power setting.	



:POWer:LEVel

Description	Sets or queries the CP mode % level (percentage of the Set power value) when the dynamic mode units are set to Percent.	
Syntax	:POWer:LEVel {<NRf> MINimum MAXimum }	
Query Syntax	:POWer:LEVel?	
Related Commands	:POWer:Set	
Parameter	<NRf> MINIMUM or MIN MAXIMUM or MAX	“% level” power value Minimum % power level Maximum % power level
Return parameter	<NR2>	Returns the “% level” current value.
Example	:POWer:LEVel MIN Sets the % level power value to the minimum.	
Query example	:POWer:LEVel? >50 Returns the “% Level” as 50 percent.	

Set →

→ Query

:POWer:T1

Description	Sets the T1 timer settings for the CP dynamic mode.	
Syntax	:POWer:T1 {<NRf>[s] MINimum MAXimum}	
Query Syntax	:POWer:T1?	
Related Commands	:POWer:T2	
Parameter	<NRf>[s] MINIMUM or MIN MAXIMUM or MAX	T1 timer setting in seconds Minimum time Maximum time
Return parameter	<NR2>	Returns the T1 timer time in s.
Example	:POWer:T1 0.200 Sets the T1 timer time to 200ms.	

Query example :POWer:T1?
>0.200
Returns the T1 timer time as 200ms.

Set →


→ Query

:POWer:T2

Description	Sets the T2 timer settings for the CP dynamic mode.	
Syntax	:POWer:T2 {<NRf>[s] MINimum MAXimum}	
Query Syntax	:POWer:T2?	
Related Commands	:POWer:T1	
Parameter	<NRf>[s] MINIMUM or MIN MAXIMUM or MAX	T2 timer setting in seconds Minimum time Maximum time
Return parameter	<NR2>	Returns the T2 timer time in ms.

Example :POWer:T2 0.200
Sets the T2 timer time to 200ms.

Query example :POWer:T2?
>0.200
Returns the T2 timer time as 200ms.



:POWer:FREQUency

Description Sets the CP dynamic mode switching frequency. This command along with the “:POWer:Duty” command is used when the dynamic time setting is set to “Freq./Duty”.
This command is only applicable for dynamic mode.

Syntax :POWer:FREQUency {<NRf> | MINimum | MAXimum}

Query Syntax :POWer:FREQUency?

Related Commands :POWer:DUTY

Parameter	<NRf>	Sets the switching frequency in hertz.
	MINIMUM or MIN	Minimum frequency
	MAXIMUM or MAX	Maximum frequency

Return parameter <NR2>
Returns the frequency in hertz.

Example :POWer:FREQUency 60
Sets the frequency to 60Hz.

Query example :POWer:FREQUency?
>60
Returns the switching frequency (60Hz).

Set →

→ Query

:POWer:DUTY

Description Sets the duty cycle for the CP dynamic mode switching frequency. This command along with the “:POWer:FREQuency” command is used when the dynamic time setting is set to “Freq./Duty”.

This command is only applicable for dynamic mode.

Syntax :POWer:DUTY {<NRf> | MINimum | MAXimum}

Query Syntax :POWer:DUTY?

Related Commands :POWer:FREQuency

Parameter	<NRf> MINIMUM or MIN MAXIMUM or MAX	Sets the duty as a percentage. Minimum duty Maximum duty
------------------	---	--

Return parameter	<NR2>	Returns the duty as a percentage.
-------------------------	-------	-----------------------------------

Example :POWer:DUTY 50

Sets the duty to 50%.

Query example :POWer:DUTY?
>50


Returns the duty (50%).

Function Commands



:PROGram:STATe	102
:PROGram	103
:PROGram[:RECall]:DEFault	104
:PROGram:START	104
:PROGram:STEP	105
:PROGram:MEMory	105
:PROGram:RUN	105
:PROGram:ONTime	106
:PROGram:OFFTime	106
:PROGram:PFTime	107
:PROGram:STIME	107
[:PROGram]:CHAIin:START	108
[:PROGram]:CHAIin	108
[:PROGram]:CHAIin:P2P	110
[:PROGram]:CHAIin[:RECall]:DEFault	110
:PROGram:SAVE	111
:NSEquence:STATe	111
:NSEquence	112
:NSEquence:START	113
:NSEquence:NUMBer	114
:NSEquence:MEMO	114
:NSEquence:MODE	115
:NSEquence:RANGe	115
:NSEquence:LOOP	116
:NSEquence:LLOad	116
:NSEquence:LAST	117
:NSEquence:CHAIin	117
:NSEquence:EDIT	118
:NSEquence:EDIT:POINt	119
:NSEquence:EDIT:END?	120
:NSEquence[:DELet]:ALL	120
:NSEquence:SAVE	120
:FSEquence:STATe	120
:FSEquence	121
:FSEquence:MEMO	122
:FSEquence:MODE	123
:FSEquence:RANGe	123
:FSEquence:LOOP	124
:FSEquence:TBASE	124
:FSEquence:LLOad	125

:FSEquence:LAST125
 :FSEquence:RPTStep126
 :FSEquence:EDIT126
 :FSEquence:EDIT:POINT127
 :FSEquence:EDIT:END?128
 :FSEquence[:DELet]:ALL128
 :FSEquence[:EDIT]:FILL128
 :FSEquence:SAVE129

:PROGrama:STATe



Description	Sets or queries the state of the program function.	
Syntax	:PROGrama:STATe {ON OFF PAUSe CONTInue NEXT}	
Query Syntax	:PROGrama:STATe? {{ON,STOP RUN PAUSe} OFF}	
Parameter	ON	Turn program on
	OFF	Program off
	PAUSe	Program pause
	RUN	Program running
	NEXT	Next step in the program
	CONTInue	Program continue
Return Parameter	ON,STOP	Program is on, stopped
	ON,PAUSE	Program is paused
	ON,RUN	Program is running
	OFF	Program is off
Example	:PROGrama:STATe ON Turns “Program” on.	
Query example	:PROGrama:STATe? >OFF “Program” is off.	



:PROGram

Description	Configures the parameters for the Program sequence. This remote command is equivalent to all the settings in the “Timing Edit for Program” menu when entering the FUNC>PROGRAM menu.	
Syntax	:PROGram {<NR1>,<NR1>,<NR1>,SKIP AUTO MANual,<NR2>,<NR2> OFF,<NR2> OFF,<NR2> OFF}	
Query Syntax	:PROGram?	
Related Commands	:PROGram:STATe	
Parameter	Parameters (In order) <NR1> <NR1> <NR1> SKIP AUTO MANual <NR2> <NR2> OFF <NR2> OFF <NR2> OFF	Description Program number (1~16) Step number (1~16) Memory number (1~256) Run parameter: On-Time (0.1~60)s Off-Time (0.1~60)s P/F Time (0.0~119.9)s Short-Time (0.1 ~ On-Time)s
Return parameter	<string>	Returns the program settings in the following order: Program: <NR1>; Start: <NR1>, Step:XX, Memory: <NR1>, Run: Skip Automatic Manual, On-Time:<NR2>, Off-Time: <NR2> OFF, P/F-Time: <NR2> OFF, Short-Time: <NR2> OFF

Example :PROGram: 1,1,1,AUTO,2.0,OFF,1.0,OFF
 Sets the program settings as follows: Program no. = 1, Step no. = 1, memory number = M001, Run = AUTO, On-Time = 2.0 secs, Off-Time = OFF, P/F Time = 1.0 secs, Short-Time = OFF.

Query example :PROGram?
 >Start:1, Step:1, Memory:1, Run:Manual, On-Time:2.0, Off-Time:0.0, P/F-Time:0.0, Short-Time:0.0
 Returns the program settings for program number 1, at step 1.

:PROGram[:RECall]:DEFault (Set) →

Description The default settings for the program sequence function.

Syntax :PROGram[:RECall]:DEFault

Example :PROGram:DEFault

(Set) →

:PROGram:STARt → (Query)

Description Sets or queries the program number for the program sequence.

Syntax :PROGram:STARt {<NR1>}

Query Syntax :PROGram:STARt?

Parameter <NR1> (1~16) program number

Return Parameter <string> Start:<NR1>

Example :PROGram:STARt 1
 Sets the program number to 1.

Query example :PROGram:STARt?
 >Start:1
 Returns the program number (1).


		Set →
		→ Query
:PROGram:STEP		
Description	Sets or queries the step number for the program sequence.	
Syntax	:PROGram:STEP {<NR1>}	
Query Syntax	:PROGram:STEP?	
Parameter	<NR1>	(1~16) step number
Return Parameter	<string>	Step:<NR1>
Example	:PROGram:STEP 1 Sets the step number to 1.	
Query example	:PROGram:STEP? >Step:1 Returns the step number (1).	

		Set →
		→ Query
:PROGram:MEMory		
Description	Sets or queries the memory number for the program sequence.	
Syntax	:PROGram:MEMory{<NR1>}	
Query Syntax	:PROGram:MEMory?	
Parameter	<NR1>	(1~256) memory number
Return Parameter	<string>	Memory:M <NR1>
Example	:PROGram:MEMory 1 Sets the memory number to 1.	
Query example	:PROGram:MEMory? >Memory:M 1 Returns the memory number (1).	


		Set →
		→ Query
:PROGram:RUN		
Description	Sets or queries the “Run” state for the selected program step in the program sequence.	

Syntax	:PROGram:RUN {SKIP AUTO MANual}	
Query Syntax	:PROGram:RUN? { Run:Skip Automatic Manual}	
Parameter	SKIP	Sets the run state to skip
	AUTO	Sets the run state to automatic
	MANual	Sets the run state to manual
Return Parameter	Run:Skip	Run state = Skip
	Run:Automatic	Run state = Automatic
	Run:Manual	Run state = Manual
Example	:PROGram:RUN SKIP Skips the selected step.	
Query example	:PROGram:RUN? >Run:Skip Returns the "Run" state (skip).	

:PROGram:ONTime



Description	Sets or queries the On-Time for the selected step number. Resolution 0.1 seconds.	
Syntax	:PROGram:ONTime {<NR2>[s]}	
Query Syntax	:PROGram:ONTime?	
Parameter	<NR2>[s]	(0.1~60) On-Time in seconds
		Turns the On-Time off.
Return Parameter	<string>	On-Time: <NR2>
Example	:PROGram:ONTime 1 Sets the On-Time to 1 second.	
Query example	:PROGram:ONTime? >On-Time:1.0 Returns the On-Time (1 second).	




:PROGram:OFFTime


Description	Sets or queries the Off-Time for the selected step number.	
-------------	--	--

Syntax	:PROGram:OFFTime {<NR2>[s] OFF}	
Query Syntax	:PROGram:OFFTime?	
Parameter	<NR2>[s]	(0~60) Off-Time in seconds
	OFF	Turns the Off-Time off.
Return Parameter	<string>	Off-Time:<NR2> (a time of 0.0 is equivalent to "OFF")
Example	:PROGram:OFFTime 1 Sets the Off-Time to 1 second.	
Query example	:PROGram:OFFTime? >Off-Time:1.0 Returns the Off-Time (1 second).	

:PROGram:PFTime



Description	Sets or queries the Pass/Fail-Time for the selected step number.	
Syntax	:PROGram:PFTime {<NR2>[s] OFF}	
Query Syntax	:PROGram:PFTime?	
Parameter	<NR2>[s]	(0 ~ (On-time + Off time - 0.1)) (in seconds)
	OFF	Turns the P/F-Time off.
Return Parameter	<string>	P/F-Time:<NR2>
Example	:PROGram:PFTime 1 Sets the P/F-Time to 1 second.	
Query example	:PROGram:PFTime? > P/F-Time:0.0 Returns the P/F-Time (1 second).	



:PROGram:STIME

Description	Sets or queries the Short-Time for the selected step number.	
-------------	--	--

Syntax	:PROGram:STIME {<NR2>[s] OFF}	
Query Syntax	:PROGram:STIME?	
Parameter	<NR2>[s] OFF	(0~On-Time) (in seconds) Turns the Short-Time off.
Return Parameter	<string>	Short-Time:<NR2>
Example	:PROGram:STIME 1 Sets the Short-Time to 1 second.	
Query example	:PROGram:STIME? >Short-Time:1.0 Returns the Short-Time (1 second).	

Set →
 ← Query

[[:PROGram]:CHAIIn:START		
Description	Sets or queries the first program number for the chain.	
Syntax	[:PROGram]:CHAIIn:START {<NR1>}	
Query Syntax	[:PROGram]:CHAIIn:START?	
Parameter	<NR1>	(1~16) Program number
Return Parameter	<string>	P1 ~ P16
Example	:CHAIIn:START 1 Sets program 1 as the start of the program chain.	
Query example	:CHAIIn:START? >P1 Returns the program number that starts the chain.	

Set →
 ← Query

[[:PROGram]:CHAIIn		
Description	Sets or queries which programs are added to program chain and the order of those programs in the program chain.	

Syntax [:PROGram]:CHAIIn
 {<NR1>|OFF, <NR1>|OFF, <NR1>|OFF, <NR1>|OFF,
 <NR1>|OFF, <NR1>|OFF, <NR1>|OFF, <NR1>|OFF,
 <NR1>|OFF, <NR1>|OFF, <NR1>|OFF, <NR1>|OFF,
 <NR1>|OFF, <NR1>|OFF, <NR1>|OFF, <NR1>|OFF}

Query Syntax [:PROGram]:CHAIIn?

Parameter	Parameters in order:	Description
	<NR1> OFF	(1~16) Program no. that follows P01.
	<NR1> OFF	(1~16) Program no. that follows P02.
	<NR1> OFF	(1~16) Program no. that follows P03.
	<NR1> OFF	(1~16) Program no. that follows P04.
	<NR1> OFF	(1~16) Program no. that follows P05.
	<NR1> OFF	(1~16) Program no. that follows P06.
	<NR1> OFF	(1~16) Program no. that follows P07.
	<NR1> OFF	(1~16) Program no. that follows P08.
	<NR1> OFF	(1~16) Program no. that follows P09.
	<NR1> OFF	(1~16) Program no. that follows P10.
	<NR1> OFF	(1~16) Program no. that follows P11.
	<NR1> OFF	(1~16) Program no. that follows P12.
	<NR1> OFF	(1~16) Program no. that follows P13.
	<NR1> OFF	(1~16) Program no. that follows P14.
	<NR1> OFF	(1~16) Program no. that follows P15.
	<NR1> OFF	(1~16) Program no. that follows P16.

Return Parameter <string> P1->XX;P2->XX;P3->XX;P4->XX;
 P5->XX;P6->XX;P7->XX;P8->XX;
 P9->XX;P10->XX;P11->XX;P12->XX;
 P13->XX;P14->XX;P15->XX;P16->XX

Where XX = P1 ~ P16 or OFF

Example :CHAIIn 4, OFF, OFF, 5, 6, OFF, OFF, OFF, OFF, OFF, OFF,
 OFF, OFF, OFF, OFF, OFF

Configures the program chain as follows:

P01 → P04 → P05 → P06 → OFF

Query example :CHAIIn?
 >P1->P4;P2->Off;P3->Off;P4->P5;P5->P6;P6->Off;
 P7->Off;P8->Off;P9->Off;P10->Off;P11->Off;
 P12->Off;P13->Off;P14->Off;P15->Off;P16->Off

Returns the program chain configuration.

[[:PROGram]:CHAIIn:P2P (Set) →
→ (Query)

Description	Sets or queries a single link in the program chain.	
Syntax	[:PROGram]:CHAIIn:P2P {<NR1>,<NR1> OFF}	
Query Syntax	[:PROGram]:CHAIIn:P2P? {P1 P2 P3 P4 P5 P6 P7 P8 P9 P10 P11 P12 P13 P14 P15 P16}	
Parameter	Parameters in order: <NR1> <NR1> OFF	Description (1~16) Program number of single link. (1~16) Program number that follows.
Query Parameter	P1 ~ P16	The program number of the first link of the chain that you are inquiring about.
Return Parameter	PX->PX Off	Returns the program number that follows or Off.

Example :CHAIIn:P2P 4,6
 Configures the program number 6 to follow after program number 4:
 P04→P06

Query example :CHAIIn:P2P? P4
 >P4->6
 Indicates that program 6 follows from program 4 in the chain.

[[:PROGram]:CHAIIn[:RECall]:DEFault (Set) →

Description	Recalls the default settings for the program chain.
Syntax	[:PROGram]:CHAIIn[:RECall]:DEFault
Example	:CHAIIn:DEFault

:PROGram:SAVE

Set →



Description	Saves the program chain.
Syntax	:PROGram:SAVE
Example	:PROG:SAVE

:NSEquence:STATe

Set →

→ Query

Description	Sets or queries the state of the Normal Sequence function.	
Syntax	:NSEquence:STATe {OFF ON PAUSE CONTINUE NEXT}	
Query Syntax	:NSEquence:STATe? {ON,STOP RUN PAUSE} OFF	
Parameter	OFF	Normal sequence Off
	ON	Normal sequence On
	PAUSE	Pause sequence
	CONTINUE	Continue sequence
	NEXT	Go to next sequence
Return Parameter	ON,STOP	Sequence has stopped
	ON, RUN	Sequence is running
	ON, PAUSE	Sequence is paused
	OFF	Sequence is off
Example	:NSEquence:STATe ON Turns “Normal Sequence” on.	
Query example	:NSEquence:STATe? >OFF “Normal Sequence” is off.	



:NSEquence

Description	Configures the parameters for the Normal Sequence. This remote command is equivalent to the all the settings in the “Timing Edit for Normal Sequence” menu when entering the FUNC>Sequence>Normal Sequence menu.	
Note	CR mode unit = mS	
Syntax	:NSEquence { <NR1>,<NR1>,<string>,CC CR CV CP,ILVL IMVL IHVL ILVH IMVH IHVH,<NR1> INFinity,<bool> OFF ON,<NR2>,<NR1> OFF}	
Query Syntax	:NSEquence?	
Related Commands	:NSEquence:STATe	
Parameter	Parameter in order: <NR1> <NR1> <string> CC CR CV CP ILVL IMVL IHVL ILVH IMVH IHVH <NR1> INFinity <bool> ON OFF <NR2> <NR1> OFF	Description Starting sequence number Current sequence number Memo message. (need to enclose in quotes) Mode Range Sets the loop number Last Load 0=Off, 1=On. Sets the load condition after the end of the sequence. Last value: Sets the value of the load condition if Last Load = On Chain: Sets the next sequence in the chain.

Return parameter	<string>	Returns the normal sequence settings in the following order: Start:<NR1>, Seq No:<NR1>, Memo:<string>, Mode:CC CR CV CP, Range:ILVL IMVL IHVL ILVH IMVH IHVH, Loop:<NR1>, Last Load: OFF ON, Last:<NR2>, Chain:<NR1>
------------------	----------	---

Example :NSEquence: 1,1,"hi",CC,ILVL,1,ON,0.000,2
Sets the normal sequence configuration to that shown below.

Query example :NSEquence:?
> Start:1, Seq No:1, Memo: HI, Mode:CC, Range:IHVL, Loop:1, Last Load:ON, Last:0.000, Chain:2
Returns the normal sequence settings.



Description Sets or queries the starting sequence number.

Syntax :NSEquence:START {<NR1>}

Query Syntax :NSEquence:START?

Parameter <NR1> (1~10) sequence number

Return Parameter <string> Start:<NR1>

Example :NSEquence:START 1
Sets the starting sequence number to 1.

Query example :NSEquence:START?
>Start:1
Returns the starting sequence number (1).

Set →

→ Query

:NSEquence:NUMBER

Description	Sets or queries the current sequence number for the normal sequence.	
Syntax	:NSEquence:NUMBER {<NR1>}	
Query Syntax	:NSEquence:NUMBER?	
Parameter/	<NR1>	(1~10) sequence number
Return Parameter	<string>	Seq No:<NR1>
Example	:NSEquence:NUMBER 1 Sets the sequence number to 1.	
Query example	:NSEquence:NUMBER? >Seq No:1 Returns the sequence number (1).	

Set →

→ Query

:NSEquence:MEMO

Description	Sets or queries the memo string for the normal sequence.	
Syntax	:NSEquence:MEMO {<string>}	
Query Syntax	:NSEquence:MEMO?	
Parameter	<string>	ASCII character string max of 12 characters. First character must be an alpha character. String must be enclosed in quotes.
Return Parameter	<string>	Memo: <string>
Example	:NSEquence:MEMO "HI" Sets the memo string to "HI".	
Query example	:NSEquence:MEMO? >Memo: HI Returns the memo string.	





:NSEquence:MODE

Description Sets or queries the mode used for the normal sequence.

Syntax :NSEquence:MODE {CC|CR|CV|CP}

Query Syntax :NSEquence:MODE?

Parameter	CC	Constant current mode
	CR	Constant resistance mode
	CV	Constant voltage mode
	CP	Constant power mode

Return Parameter <string> Mode: CC|CR|CV|CP

Example :NSEquence:MODE CC
Sets the mode to CC.

Query example :NSEquence:MODE?
>Mode: CC
Returns the mode.





:NSEquence:RANGe

Description Sets or queries the range used for the normal sequence.

Syntax :NSEquence:RANGe
{ ILVL|IMVL|IHVL|ILVH|IMVH|IHVH }

Query Syntax :NSEquence:RANGe?

Parameter	ILVL	Low I range, low V range
	IMVL	Middle I range, low V range
	IHVL	High I range, low V range
	ILVH	Low I range, high V range
	IMVH	Middle I range, high V range
	IHVH	High I range, high V range

Return Parameter <string> Returns the range in the following format:
Range: ILVL

Example :NSEquence:RANGe IHVL
Sets the range to IHVL.

Query example :NSEquence:RANGe?
>Range: IHVL
Returns the range.

Set →

→ Query

:NSEquence:LOOP

Description Sets or queries the number of loops for the sequence.

Syntax :NSEquence:LOOP {<NR1>|INFINITY}

Query Syntax :NSEquence:LOOP?

Parameter	<NR1> INFINITY	(1~9999) Sets the number of loops Sets the number of loops to infinite.
-----------	-------------------	--

Return Parameter	<string>	Returns the number of loops in the following format: Loop: <NR1> Infinity
------------------	----------	--

Example :NSEquence:LOOP 1
Sets the number of loops to 1.

Query example :NSEquence:LOOP?
>Loop: 1
Returns the number of loops(1).

Set →

→ Query

:NSEquence:LLOad

Description Sets or queries the Last Load state.

Syntax :NSEquence:LLOad {<bool>|ON|OFF}


Query Syntax :NSEquence:LLOad?

Parameter	ON, 1 OFF, 0	Turns Last Load on. Turns Last Load off.
-----------	-----------------	---

Return Parameter	<string>	Returns the Last Load state in the following format: Last Load:ON OFF
------------------	----------	--

Example :NSEquence:LLOad ON
Turns Last Load on.

Query example :NSEquence:LLOad?
>Last Load: ON
Returns the last load state.



:NSEquence:LAST

Description Sets or queries the value of Last Load when Last Load = ON. The unit depends on the Mode.

Note CR mode unit = mS

Syntax :NSEquence:LAST {<NR2>}


Query Syntax :NSEquence:LAST?

Parameter <NR2> current value(CC), resistance value(CR), voltage value(CV), power value(CP).

Return Parameter <string> Returns the value for the Last Load in the following format:
Last:<NR2>

Example :NSEquence:LAST 1.000
Sets the value of Last Load to 1.000.

Query example :NSEquence:LAST?
>Last: 1.000
Returns the value of Last Load.



:NSEquence:CHAin

Description Sets or queries the next sequence in the chain.

Syntax :NSEquence:CHAin {<NR1>|OFF}


Query Syntax :NSEquence:CHAin?

Parameter	<NR1>	The sequence number of the next sequence in the chain.
	OFF	End the chain at the current sequence.

Return Parameter	<code><string></code>	Returns the next sequence in the chain in the following format: Chain: <code><NR1></code> OFF
------------------	-----------------------------	---

Example	:NSEquence:CHAI n 2 Sets the next sequence in the chain as S02.
---------	--

Query example	:NSEquence:CHAI? >Chain: 2 Returns the next sequence in the chain (S02).
---------------	--



:NSEquence:EDIT

Description	Configures the parameters for the Data Edit for Normal Sequence menu, equivalent to entering the FUNC>Sequence>Normal Sequence>Data Edit menu.
-------------	--

Note	CR mode unit = mS
------	-------------------

Syntax	:NSEquence:EDIT {<NR1>,<NR1>,<NR2>,<NR1>,<NR1>,<NR1>,<NR1> ,<bool> OFF ON,<bool> OFF ON,<bool> OFF ON, <bool> OFF ON}
--------	--

Query Syntax	:NSEquence:EDIT?
--------------	------------------

Related Commands	:NSEquence:
------------------	-------------

Parameter	Parameters in order:	Description
	<code><NR1></code>	Current step number
	<code><NR1></code>	Total number of steps
	<code><NR2></code>	Value
	<code><NR1></code>	Time: hours
	<code><NR1></code>	Time: minutes
	<code><NR1></code>	Time: seconds
	<code><NR1></code>	Time: milliseconds
	<code><bool></code> OFF ON	LOAD setting
	<code><bool></code> OFF ON	TRIG OUT setting
	<code><bool></code> OFF ON	RAMP setting
	<code><bool></code> OFF ON	PAUSE setting

Return parameter	<string>	Returns the settings for the Data Edit for Normal Sequence menu: Step: <NR1>/<NR1>, Value: <NR1>, Time: <NR1>H: <NR1>M: <NR1>S: <NR1>ms, LOAD:ON OFF, TRIG OUT:ON OFF, RAMP: ON OFF, PAUSE: ON OFF
------------------	----------	---

Example :NSEquence:EDIT 3,12,0.1,0,1,0,0,ON,OFF,OFF,ON
Configures the Data Edit for Normal Sequence menu to the settings shown below.

Query example :NSEquence:EDIT?
> Step:3/12, Value:0.10000, Time:0H:0M:1S:0ms,
LOAD:ON, TRIG OUT:OFF, RAMP:OFF, PAUSE:ON

:NSEquence:EDIT:POINTt 

Description Sets or queries the current point in the sequence.

Syntax :NSEquence:EDIT:POINTt {<NR1>}

Query Syntax :NSEquence:EDIT:POINTt?

Related Commands :NSEquence:EDIT:END?

Parameter/ Return parameter	<NR1>	1~1000*. The current point in the sequence. *Depends on the number of steps in the sequence.
--------------------------------	-------	--

Example :NSEquence:EDIT:POINTt 10
Sets the current point to 10.

Query example :NSEquence:EDIT:POINTt?
>10
Returns the current point in the sequence.

:NSEquence:EDIT:END? → (Query)

Description	Returns the number of points in the sequence.	
Query Syntax	:NSEquence:EDIT:END?	
Return parameter	<NR1>	1~1000
Query example	:NSEquence:EDIT:END? > 20 Indicates that there are 20 steps in the sequence.	

:NSEquence[:DELEt]:ALL (Set) →

Description	Deletes all the data points for the normal sequence.	
Syntax	:NSEquence[:DELEt]:ALL	
Example	:NSEquence:ALL	

:NSEquence:SAVE (Set) →

Description	Saves the data points for the normal sequence.	
Syntax	:NSEquence:SAVE	
Example	:NSEquence:SAVE	


:FSEquence:STATe (Set) →
→ (Query)

Description	Sets or queries the state of the Fast Sequence function.	
Syntax	:FSEquence:STATe {ON OFF}	
Query Syntax	:FSEquence:STATe?	
Parameter	ON OFF	Turn fast sequence on Turn fast sequence off
Return Parameter	ON,STOP RUN,STOP OFF	Fast sequence is on Fast sequence is running Fast sequence is off

Example :FSEquence:STATe ON
Turns “Fast Sequence” on.

Query example :FSEquence:STATe?
>OFF
“Fast Sequence” is off.

:FSEquence



Description Configures the parameters for the Fast Sequence. This remote command is equivalent to all the settings in the “Timing Edit for Fast Sequence” menu when entering the FUNC>Sequence>Fast Sequence menu.

Note CR mode unit = mS

Syntax :FSEquence {<string>,CC|CR, ILVL|IMVL||IHVL|ILVH|IMVH|IHVH, <NR1>|INFinity,<NR2>,<bool>|OFF|ON,<NR2>,<NR1>}

Query Syntax :FSEquence?

Related Commands :FSEquence:STATe

Parameter	Parameter in order:	Description
	<string>	Memo message. (Need to enclose in quotes)
	CC CR	Mode
	ILVL IMVL IHVL ILVH IMVH IHVH	Range
	<NR1> INFinity	Number of loops
	<NR2>	Time base in seconds
	<bool> ON OFF	Last Load 0=Off, 1=On. Sets the load condition after the end of the sequence.
	<NR2>	Last value: Sets the value of the load condition for Last Load = On

	<NR1>	Repeat Step from (0001~1000) per loop
Return parameter	<string>	Returns the fast sequence settings in the following order: FSeq:ON OFF; Memo:<string>, Mode: CC CR, Range: ILVL IMVL IHVL ILVH IMVH IHVH, Loop: <NR1> Infinity, Time Base:<NR2>, Last Load:ON OFF, Last:<NR2>, RPTSTEP:<NR1>

Example :FSEquence HI,CC,ILVL,5,0.3,1,0.7,11
Sets the fast sequence configuration to that shown below.

Query example :FSEquence?
>Memo: HI, Mode:CC, Range:ILVL, Loop:5, Time Base:300.00, Last Load:OFF, Last:0.70000, RPTSTEP:11
Returns the fast sequence settings.

:FSEquence:MEMO 

Description Sets or queries the memo string for the fast sequence.

Syntax :FSEquence:MEMO {<string>}

Query Syntax :FSEquence:MEMO?


Parameter <string> ASCII character string max of 12 characters. First character must be an alpha character. The string must be enclosed in quotes.

Return Parameter <string> Memo:<string>

Example :FSEquence:MEMO "HI"
Sets the memo string to "HI".

Query example :FSEquence:MEMO?
>Memo: HI
Returns the memo string.

:FSEquence:MODE



Description Sets or queries the mode used for the fast sequence.

Syntax :FSEquence:MODE {CC|CR}


Query Syntax :FSEquence:MODE?

Parameter	CC	Constant current mode
	CR	Constant resistance mode

Return Parameter <string> Mode: CC|CR

Example :FSEquence:MODE CC
Sets the mode to CC.

Query example :FSEquence:MODE?
>Mode: CC
Returns the mode.



:FSEquence:RANGe

Description Sets or queries the range used for the fast sequence.

Syntax :FSEquence:RANGe
{ ILVL|IMVL|IHVL|ILVH|IMVH|IHVH }


Query Syntax :FSEquence:RANGe?

Parameter	ILVL	Low I range, low V range
	IMVL	Middle I range, low V range
	IHVL	High I range, low V range
	ILVH	Low I range, high V range
	IMVH	Middle I range, high V range
	IHVH	High I range, high V range

Return Parameter	<string>	Returns the range in the following format: Range: ILVL
------------------	----------	---

Example	:FSEquence:RANGe IHVL Sets the range to IHVL.
---------	--

Query example	:FSEquence:RANGe? >Range: IHVL Returns the range.
---------------	---



:FSEquence:LOOP

Description	Sets or queries the number of loops for the sequence.
-------------	---

Syntax	:FSEquence:LOOP {<NR1> INFinity}
--------	----------------------------------


Query Syntax	:FSEquence:LOOP?
--------------	------------------

Parameter	<NR1>	(1~9999) Sets the number of loops
	INFinity	Sets the number of loops to infinite.

Return Parameter	<string>	Loop:<NR1>
------------------	----------	------------

Example	:FSEquence:LOOP 1 Sets the number of loops to 1.
---------	---

Query example	:FSEquence:LOOP? >Loop:1 Returns the number of loops(1).
---------------	--



:FSEquence:TBASE

Description	Sets or queries the Time Base.
-------------	--------------------------------

Syntax	:FSEquence:TBASE {<NR2>[s]}
--------	-----------------------------

Query Syntax	:FSEquence:TBASE?
--------------	-------------------


Parameter	<NR2>[s]	0.000025 ~ 0.6s
-----------	----------	-----------------

Return Parameter	<string>	Returns the Time Base in the following format: Time Base:<NR2>
------------------	----------	---

Example :FSEquence:TBASe 0.3
Sets the time base to 300ms.

Query example :FSEquence:TBASe?
>Time Base:0.30000
Returns the time base.

:FSEquence:LLOad



Description Sets or queries the Last Load state.

Syntax :FSEquence:LLOad {<bool>ON|OFF}


Query Syntax :FSEquence:LLOad?

Parameter	ON, 1	Turns Last Load on.
	OFF, 0	Turns Last Load off.

Return Parameter	<string>	Last Load:ON OFF
------------------	----------	------------------

Example :FSEquence:LLOad ON
Turns Last Load on.

Query example :FSEquence:LLOad?
>Last Load: ON
Returns the last load state.



:FSEquence:LAST

Description Sets or queries the value of Last Load when Last Load = ON.

Note CR mode unit = mS

Syntax :FSEquence:LAST{<NR2>}

Query Syntax :FSEquence:LAST?

Parameter	<NR2>	Current value(CC), resistance value(CR), voltage value(CV), power value(CP).
-----------	-------	--

Return Parameter	<string>	Last:<NR2>
------------------	----------	------------

Example :FSEquence:LAST 1.000
Sets the value of Last Load to 1.000.

Query example :FSEquence:LAST?
 >Last: 1.000
 Returns the value of Last Load.

Set →

:FSEquence:RPTStep

→ Query

Description	Sets or queries the last step number per loop.	
Syntax	:FSEquence:RPTStep {<NR1>}	
Query Syntax	:FSEquence:RPTStep?	
Parameter	<NR1>	1~1000
Return Parameter	<string>	RPTSTEP:<NR1>
Example	:FSEquence:RPTStep 11 Sets the RPTSTEP to 11.	


Query example :FSEquence:RPTStep?
 > RPTSTEP: 11
 Returns the RPTSTEP number.

Set →

:FSEquence:EDIT

→ Query

Description	Configures the parameters for the Data Edit for Fast Sequence menu, equivalent to entering the FUNC>Sequence>Fast Sequence>Edit Sequence menu.	
Note	CR mode unit = mS	
Syntax	:FSEquence:EDIT {<NR1>,<NR1>,<NR2>,<bool> OFF ON}	
Query Syntax	:FSEquence:EDIT?	
Related Commands	:FSEquence:	

Parameter	Parameters in order: <NR1> <NR1> <NR2> <bool> OFF ON	Description
Return parameter	<string>	Returns the settings for the Data Edit for Fast Sequence menu: Step:<NR1>/<NR1>, Value:<NR2>, TRIG OUT:ON OFF
Example	:FSEquence:EDIT 4,11,0.1,OFF Configures the Data Edit for Normal Sequence menu to the settings shown below.	
Query example	:FSEquence:EDIT? > Step:0004/0011; Value:0.10000, TRIG OUT:OFF	
		
	:FSEquence:EDIT:POINTt	
Description	Sets or queries the current point in the sequence.	
Syntax	:FSEquence:EDIT:POINTt {<NR1>}	
Query Syntax	:FSEquence:EDIT:POINTt?	
Related Commands	:FSEquence:EDIT:END?	
Parameter/ Return parameter	<NR1>	1~1000*. The current point in the sequence. *Depends on the number of steps in the sequence.
Example	:FSEquence:EDIT:POINTt 10 Sets the current point to 10.	
Query example	:FSEquence:EDIT:POINTt? >10 Returns the current point in the sequence.	

:FSEquence:EDIT:END? → (Query)

Description	Returns the number of points in the sequence.	
Query Syntax	:FSEquence:EDIT:END?	
Return parameter	<NR1>	1~1000
Query example	:FSEquence:EDIT:END? > 20 Indicates that there are 20 steps in the sequence.	

:FSEquence[:DELet]:ALL (Set) →

Description	Deletes all the data points for the fast sequence.	
Syntax	:FSEquence[:DELet]:ALL	
Example	:FSEquence:ALL	

:FSEquence[:EDIT]:FILL (Set) →
→ (Query)

Description	The FILL function is used to evenly fill up the current or resistance value settings from a starting step to a finishing step. This function is equivalent to entering the FUNC>Sequence>Fast Sequence>Edit Sequence>Fill menu.	
Note	CR mode unit = mS	
Syntax	:FSEquence[:EDIT]:FILL {<NR2>,<NR2>,<NR1>,<NR1>}	
Query Syntax	:FSEquence[:EDIT]:FILL?	
Related Commands	:FSEquence:EDIT	

Parameter	Parameters in order:	Description
	<NR2> <NR2> <NR1> <NR1>	Start_Value End_Value Start_Step End_Step
Return parameter	<string>	Returns the settings for the Fill Edit for Fast Sequence menu: Start Value:<NR2>, End Value:<NR2>, Start Step:<NR1>, End Step:<NR1>

Example :FSEquence:FILL 0.1,0.5,1,159
Fills the values of step 1 to step 159 gradually from 0.1A to 0.5A.

Query example :FSEquence:FILL?
>Start Value:0.10000, End Value:0.50000, Start Step:1, End Step:159

:FSEquence:SAVE (Set) →

Description Saves the data points for the fast sequence.


Syntax :FSEquence:SAVE

Example :FSEquence:SAVE

Utility Commands

:UTILITY:SYSTEM?	130
:UTILITY:LOAD	131
:UTILITY:LOAD:MODE	132
:UTILITY:LOAD:RANGE	132
:UTILITY:INTERFACE	133
:UTILITY:BRATE	133
:UTILITY:SBIT	134
:UTILITY:PARITY	134
:UTILITY:TIME	135
:UTILITY:KNOB	135
:UTILITY:SPEAKER	136
:UTILITY:ALARM	136
:UTILITY:UNREG	137
:UTILITY:GNG	137
:UTILITY:CONTRAST	138
:UTILITY:BRIGHTNESS	138
:UTILITY:LANGUAGE	138
:UTILITY:REMOTE	139
:UTILITY:REMOTE:MODE	139

:UTILITY:SYSTEM?



Description	Returns the manufacturer, model, serial number and firmware version number.	
Query Syntax	:UTILITY:SYSTEM?	
Return parameter	<string>	model name, serial number, firmware version
Query example	:UTILITY:SYSTEM? >GW,PEL-3041,00000001,V1.01.010 Returns the system information.	

Set →

← Query

:UTILity:LOAD

Description	Sets or queries the Auto Load and Auto Load On settings. This is equivalent to the settings in the Shift+UTILITY>Load menu.	
Syntax	:UTILity:LOAD {OFF ON LOAD PROG NSEQ FSEQ}	
Query Syntax	:UTILity:LOAD?	
Parameter	OFF ON LOAD PROG NSEQ FSEQ	Turns Auto Load off. Turns Auto Load on. This will turn the load on automatically at start up. The type of load function that is automatically turned on is configured below. Configure the load to automatically turn on in CC, CR, CV or CP mode. Configure the load to automatically turn on a program sequences. Configure the load to automatically turn on a normal sequence. Configure the load to automatically turn on a fast sequence.
Return Parameter	<string>	Load:On Off, Load On:Load Prog NSeq FSeq
Example	:UTILity:LOAD ON FSEQ Configures the unit to automatically turn fast sequences on at start up (with the load on).	
Query example	:UTILity:LOAD? > Load:On, Load On:Prog The unit is configured to automatically turn Programs on at start up (with the load on).	

Set →
 → Query

:UTILity:LOAD:MODE

Description	Sets or queries the Load Off (Mode) setting. This is equivalent to the settings in the Shift+UTILITY>Load menu.	
Syntax	:UTILity:LOAD:MODE {<bool> OFF ON}	
Query Syntax	:UTILity:LOAD:MODE?	
Parameter	OFF, 0	Sets Load Off (Mode) to OFF.
	ON, 1	Sets Load Off (Mode) to ON.
Return Parameter	OFF	Load Off (Mode) is OFF.
	ON	Load Off (Mode) is ON.
Example	:UTILity:LOAD:MODE ON Turns Load Off (Mode) to on.	
Query example	:UTILity:LOAD:MODE? > Off Load Off (Mode) is off.	

Set →
 → Query

:UTILity:LOAD:RANGe

Description	Sets or queries the Load Off (Range) setting. This is equivalent to the settings in the Shift+UTILITY>Load menu.	
Syntax	:UTILity:LOAD:RANGe {<bool> OFF ON}	
Query Syntax	:UTILity:LOAD:RANGe?	
Parameter	OFF, 0	Sets Load Off (Range) to OFF.
	ON, 1	Sets Load Off (Range) to ON.
Return Parameter	OFF	Load Off (Range) is OFF.
	ON	Load Off (Range) is ON.
Example	:UTILity:LOAD:RANGe ON Turns Load Off (Range) to on.	

Query example :UTILity:LOAD:RANGe?
 > Off
 Load Off (Range) is off.

Set →

:UTILity:INTerface

→ Query

Description Sets or queries the remote interface. Settings only take effect after restart.

Syntax :UTILity:INTerface {USB|RS232}

Query Syntax :UTILity:INTerface?

Parameter/	USB	USB remote interface
Return Parameter	RS232	RS2323 remote interface

Example :UTILity:INTerface RS232
 Sets the interface to RS232.

Query example :UTILity:INTerface?
 >RS232
 The current remote interface is RS232.

Set →

:UTILity:BRATe

→ Query

Description Sets the baud rate when the remote interface is set to RS232. Settings only take effect after restart.

Syntax :UTILity:BRATe {<NR1>}

Query Syntax :UTILity:BRATe?

Parameter/	<NR1>	2400, 4800, 9600, 19200,
Return Parameter		38400

Example :UTILity:BRATe 9600
 Sets the baud rate to 9600.

Query example :UTILity:BRATe?
 >9600
 The baud rate is 9600.

Set →

→ Query

:UTILity:SBIT

Description	Sets the number of stop bits when the remote interface is set to RS232. Settings only take effect after restart.	
Syntax	:UTILity:SBIT {<NR1>}	
Query Syntax	:UTILity:SBIT?	
Parameter/ Return Parameter	<NR1>	1, 2
Example	:UTILity:SBIT 1 Sets the stop bits to 1.	
Query example	:UTILity:SBIT? >1 Stop bits = 1.	

Set →

→ Query

:UTILity:PARity

Description	Sets the parity when the remote interface is set to RS232. Settings only take effect after restart.	
Syntax	:UTILity:PARity {NONE ODD EVEN}	
Query Syntax	:UTILity:PARity?	
Parameter/ Return Parameter	NONE ODD EVEN	No parity Odd parity Even parity
Example	:UTILity:PARity NONE The parity is set to none.	
Query example	:UTILity:PARity? >None Parity = None.	

Set →

→ Query

:UTILity:TIME

Description	Sets or queries the date and time for the unit.	
Syntax	:UTILity:TIME <NR1>,<NR1>,<NR1>,<NR1>,<NR1>	
Query Syntax	:UTILity:TIME?	
Parameter	Parameters in order <NR1> <NR1> <NR1> <NR1> <NR1>	Description Month Day Year Hour Minute
Return Parameter	<string>	Month:<NR1>, Day: <NR1>, Year: <NR1>, Hour: <NR1>, Minute: <NR1>
Example	:UTILity:TIME 10,2,2013,8,26 Sets the date to October 2, 2013. Sets the time to 8:26.	

Query example :UTILity:TIME?
> Month:10, Day:2, Year:2013, Hour:8, Minute:26

Set →

→ Query


:UTILity:KNOB

Description	<p>The Knob Type setting determines if values are updated immediately as they are edited or if they are only updated after the Enter key is pressed.</p> <p>The Updated setting is applicable for when the load is already on and the user wishes to change the set values (current, voltage, etc.) in real-time.</p> <p>The Old setting will only update the values after the Enter key is pressed.</p>	
Syntax	:UTILity:KNOB {OLD UPDated}	
Query Syntax	:UTILity:KNOB?	
Parameter/ Return Parameter	OLD UPDated	Old setting Updated setting

Example :UTILity:KNOB OLD
Sets the knob type to OLD.

Query Example :UTILity:KNOB?
>Old

:UTILity:SPEaker



Description Turns the speaker on or off.
Note: This will not turn the Go/NoGo alarm tone settings.

Syntax :UTILity:SPEaker {<bool>|ON|OFF}


Query Syntax :UTILity:SPEaker?

Parameter	ON, 1 OFF, 0	Speaker on Speaker off
Return Parameter	On Off	Speaker on Speaker off

Example :UTILity:SPEaker ON
Turns the speaker on.

Query Example :UTILity:SPEaker?
>On

:UTILity:ALARm



Description Enables/disables the alarm tone for the unit.

Syntax :UTILity:ALARm {<bool>|ON|OFF}

Query Syntax :UTILity:ALARm?

Parameter	ON, 1 OFF, 0	Alarm on Alarm off
Return Parameter	On Off	Alarm on Alarm off

Example :UTILity:ALARm ON
Enables the alarm tone.

Query Example :UTILity:ALARm?
>On

:UTILity:UNReg

Set →

→ Query

Description Enables/disables the UnReg alarm tone for the unit.

Syntax :UTILity:UNReg {<bool>|ON|OFF}

Query Syntax :UTILity:UNReg?

Parameter	ON, 1	Alarm on
	OFF, 0	Alarm off

Return Parameter	On	Alarm on
	Off	Alarm off

Example :UTILity:UNReg ON
Enables the alarm tone.

Query Example :UTILity:UNReg?
>On

Set →

→ Query

:UTILity:GNG

Description Enables/disables the Go/NoGo alarm tone for the unit.

Syntax :UTILity:GNG {<bool>|ON|OFF}

Query Syntax :UTILity:GNG?

Parameter	ON, 1	Go/NoGo alarm tone on
	OFF, 0	Go/NoGo alarm tone off

Return Parameter	On	Go/NoGo alarm tone on
	Off	Go/NoGo alarm tone off

Example :UTILity:GNG ON
Enables the Go/NoGo alarm tone.

Query Example :UTILity:GNG?
>On

Set →
 → Query

:UTILITY:CONTrast		
Description	Sets or queries the display contrast level.	
Syntax	:UTILITY:CONTrast {NR1}	
Query Syntax	:UTILITY:CONTrast?	
Parameter/ Return Parameter	<NR1>	3~13 (low ~ high)
Example	:UTILITY:CONTrast 8 Sets the contrast to 8.	
Query Example	:UTILITY:CONTrast? >8	

Set →
 → Query

:UTILITY:BRIGhtness		
Description	Sets or queries the display contrast level.	
Syntax	:UTILITY:BRIGhtness {NR1}	
Query Syntax	:UTILITY:BRIGhtness?	
Parameter/ Return Parameter	<NR1>	50~90 (low ~ high)
Example	:UTILITY:BRIGhtness 70 Sets the contrast to 70.	
Query Example	:UTILITY:BRIGhtness? >70	

Set →
 → Query

:UTILITY:LANGuage		
Description	Sets or queries the language. Note: English is the only available language.	
Syntax	:UTILITY:LANGuage {ENGLish}	
Query Syntax	:UTILITY:LANGuage?	

Parameter/ Return Parameter	ENGLISH	English language settings
--------------------------------	---------	---------------------------

Example :UTILity:LANGUage? ENGLISH
Sets the language to English.

Query Example :UTILity:LANGUage?
>English

:UTILity:REMOte

Set →

Description Turns the remote control on or off.

Syntax :UTILity:REMOte {OFF|0|ON|1}

Parameter	OFF/0	Turns Remote control off
	ON/1	Turns remote control on

Example :UTIL:REM 1
Turns remote control on.

:UTILity:REMOte:MODE

Set →

Description Sets the remote mode to fast or normal. When in fast mode, the panel interface is deactivated with an interface time of no more than 10ms. Normal mode has an interface time of 30~130ms. In normal mode the display interface continues to update the screen in real-time.

Syntax :UTILity:REMOte:MODE {NORMAL|0|FAST|1}

Parameter	NORMAL/0	NORMAL
	FAST/1	FAST

Example :UTIL:REM:MODE 1
Turns remote mode to fast.

File Commands

:MEMory:SAVE.....	140
:MEMory:RECall.....	140
:PRESet:SAVE.....	141
:PRESet:RECall	141
:SETup:SAVE.....	141
:SETup:RECall	141
:FACTory[:RECall]	142
:USER[:DEFault]:SAVE.....	142
:USER[:DEFault]:RECall	142

:MEMory:SAVE



Description Saves Memory Data to internal memory to one of 256 slots.

Syntax :MEMory:SAVE {<NR1>}

Parameter <NR1> M001 ~ M256

Example :MEMory:SAVE 1
Save Memory Data to M001.

:MEMory:RECall



Description Recalls Memory Data from internal memory to one of 256 slots.

Syntax :MEMory:RECall {<NR1>}

Parameter <NR1> M001 ~ M256

Example :MEMory:RECall 1
Recall Memory Data from M001.

:PRESet:SAVE

Description Saves Preset Data to internal memory to one of 9 slots.

Syntax :PRESet:SAVE {<NR1>}

Parameter <NR1> P1 ~ P9

Example :PRESet:SAVE 1
Save Preset Data to P1.


:PRESet:RECall

Description Recalls Preset Data from internal memory to one of 9 slots.

Syntax :PRESet:RECall {<NR1>}

Parameter <NR1> P1 ~ P9

Example :PRESet:RECall 1
Recall Preset Data from P1.


:SETup:SAVE

Description Saves Setup Data to internal memory to one of 100 slots.

Syntax :SETup:SAVE {<NR1>}

Parameter <NR1> S001 ~ S100

Example :SETup:SAVE 1
Save Setup Data to S001.

:SETup:RECall

Description Recalls Setup Data from internal memory to one of 100 slots.

Syntax :SETup:RECall {<NR1>}

Parameter <NR1> S001 ~ S100


Example :SETup:RECall 1
 Recall Setup Data from S001.

:FACTory[:RECall] 

Description Recalls the default settings. See the user manual
 for the default settings.

Syntax :FACTory[:RECall]

Example :FACTory

:USER[:DEFault]:SAVE 

Description Saves the current settings as the user default.

Syntax :USER[:DEFault]:SAVE

Example :USER:SAVE

Saves the current settings as the user default.

:USER[:DEFault]:RECall 

Description Recalls the user default settings.

Syntax :USER[:DEFault]:RECall

Example :USER:RECall

Recalls the user default settings.

SCPI Register Commands

:SYSTem:ERRor?	143
:STATus:PRESet	144
:STATus:QUEStionable:CONDition?	144
:STATus:QUEStionable:ENABle	145
:STATus:QUEStionable[:EVENT]?	145
:STATus:QUEStionable:NTRansition	146
:STATus:QUEStionable:PTRansition	147
:STATus:OPERation:CONDition?	147
:STATus:OPERation:ENABle	148
:STATus:OPERation[:EVENT]?	148
:STATus:OPERation:NTRansition	149
:STATus:OPERation:PTRansition	149
:STATus:CSUMmary:CONDition?	150
:STATus:CSUMmary:ENABle	150
:STATus:CSUMmary[:EVENT]?	151
:STATus:CSUMmary:NTRansition	151
:STATus:CSUMmary:PTRansition	152

:SYSTem:ERRor?

→ **Query**

Description Return the error message in the error queue. If there is no error, "+0, "No error." Will be returned.

Query Syntax :SYSTem:ERRor?

Return parameter <string> Error code, followed by error description.

Query example :SYSTem:ERRor?
> +0, "No error."
Returns the system information.

:STATus:PRESet



Description The :STATus:PRESet command resets the enable registers NTR/PTR registers from Operation Status, Questionable Status and CSummary Status registers.

Preset Value	Register	Preset
	Operation Status Enable	All bits set to 1
	Operation Status PTR	All bits set to 1
	Operation Status NTR	All bits set to 0
	Questionable Status Enable	All bits set to 0
	Questionable Status PTR	All bits set to 1
	Questionable Status NTR	All bits set to 0
	CSummary Status Enable	All bits set to 0
	CSummary Status PTR	All bits set to 1
	CSummary Status NTR	All bits set to 0

Syntax :STATus:PRESet

:STATus:QUEStionable:CONDition?




Description Returns the status of the Questionable Status Condition register. See page 157 for details.

Query Syntax :STATus:QUEStionable:CONDition?

Return parameter	<NR1>	Condition	<NR1>	Condition
	1	OV	512	UV
	2	OC	1024	EXT
	8	OP	2048	REV
	16	OT	All other bits	Not used

Query example :STATus:QUEStionable:CONDition?
>1

Indicates an over voltage (OV) error has occurred.

:STATus:QUEStionable:ENABle



Description Sets which events are enabled in the Questionable Status Enable register. The mask values are the bit weights of the events. See page 157 for details.

Syntax :STATus:QUEStionable:ENABle <NR1>

Query Syntax :STATus:QUEStionable:ENABle?

Parameter/ Return Parameter	<NR1>	Condition	<NR1>	Condition
	1	OV	512	UV
	2	OC	1024	EXT
	8	OP	2048	REV
	16	OT	All other bits	Not used

Example :STATus:QUEStionable:ENABle 11
 Events OV, OC and OP (Bits 1, 2, 3) are enabled in the Questionable Status Enable register.

Query example :STATus:QUEStionable:ENABle?
 >11
 Indicates that OV, OC and OP bits are enabled in the Questionable Status Enable register.

:STATus:QUEStionable[:EVENTt]? 

Description Returns the status of the Questionable Status Event register. The register is cleared upon reading. See page 157 for details.

Query Syntax :STATus:QUEStionable[:EVENTt]?

Return parameter	<NR1>	Condition	<NR1>	Condition
	1	OV	512	UV
	2	OC	1024	EXT
	8	OP	2048	REV
	16	OT	All other bits	Not used

Query example :STATus:QUEStionable:EVENT?
> 1

Indicates an over voltage (OV) event has occurred.

:STATus:QUEStionable:NTRansition

Description Determines whether a negative transition (NTR 1→0) in the Questionable Status Condition register will set the corresponding event in the Questionable Status Event register.

The mask values are the bit weights of the Questionable Status NTR filters. See page 157 for details.

Syntax :STATus:QUEStionable:NTRansition <NR1>

Query Syntax :STATus:QUEStionable:NTRansition?

Parameter/ Return Parameter	<NR1>	Condition	<NR1>	Condition
	1	OV	512	UV
	2	OC	1024	EXT
	8	OP	2048	REV
	16	OT	All other bits	Not used

Example :STATus:QUEStionable:NTRansition 11

Configures the OV, OC and OP bits (Bits 1, 2, 3) in the Questionable Status Condition register to set the corresponding bits in the Questionable Status Enable register on a negative transition

Query example :STATus:QUEStionable:NTRansition?
>11

OV, OC and OP bits are configured to NTR in the Questionable Status NTR filter.

:STATus:QUEStionable:PTRansition



Description Determines whether a positive transition (PTR 0→1) in the Questionable Status Condition register will set the corresponding event in the Questionable Status Event register.

The mask values are the bit weights of the Questionable Status PTR filters. See page 157 for details.

Syntax :STATus:QUEStionable:PTRansition <NR1>

Query Syntax :STATus:QUEStionable:PTRansition?

Parameter/ Return Parameter	<NR1>	Condition	<NR1>	Condition
	1	OV	512	UV
	2	OC	1024	EXT
	8	OP	2048	REV
	16	OT	All other bits	Not used

Example :STATus:QUEStionable:PTRansition 11

Configures the OV, OC and OP bits (Bits 1, 2, 3) in the Questionable Status Condition register to set the corresponding bits in the Questionable Status Enable register on a positive transition.

Query example :STATus:QUEStionable:PTRansition?
>11

OV, OC and OP bits are configured to PTR in the Questionable Status PTR filter.

:STATus:OPERation:CONDition? 

Description Returns the status of the Operation Status Condition register. See page 158 for details.


Query Syntax :STATus:OPERation:CONDition?

Return parameter	<NR1>	Condition	<NR1>	Condition
	1	CAL	All other bits	
	32	WTG		

Query example :STaTus:OPERation:CONDition?
>32

Indicates that the unit is waiting for a trigger.

:STaTus:OPERation:ENABLE



Description Sets which events are enabled in the Operation Status Enable register. The mask values are the bit weights of the events. See page 158 for details.

Syntax :STaTus: OPERation:ENABLE <NR1>


Query Syntax :STaTus: OPERation:ENABLE?

Parameter/ Return Parameter	<NR1>	Condition	<NR1>	Condition
1		CAL	All other	Not used
32		WTG	bits	

Example :STaTus:OPERation:ENABLE 32
WTG is enabled in the OPERATION Status Enable register.

Query example :STaTus:OPERation:ENABLE?
>32
Indicates that the WTG bit is enabled in the Operation Status Enable register.

:STaTus:OPERation[:EVENT]?



Description Returns the status of the Operation Status Event register. The register is cleared upon reading. See page 158 for details.

Query Syntax :STaTus:OPERation[:EVENT]?

Return parameter	<NR1>	Condition	<NR1>	Condition
1		CAL	All other	Not used
32		WTG	bits	

Query example :STaTus:OPERation:EVENT?
> 1
Indicates that unit is currently calibrating.

:STATus:OPERation:NTRansition



Description Determines whether a negative transition (NTR 1→0) in the Operation Status Condition register will set the corresponding event in the Operation Status Event register.

The mask values are the bit weights of the Operation Status NTR filters. See page 158 for details.

Syntax :STATus:OPERation:NTRansition <NR1>

Query Syntax :STATus:OPERation:NTRansition?

Parameter/ Return Parameter	<NR1>	Condition	<NR1>	Condition
	1	CAL	All other bits	Not used
	32	WTG		

Example :STATus:OPERation:NTRansition 1

Configures the CAL bit (Bit 1) in the Operation Status Condition register to set the corresponding bit in the Questionable Status Enable register on a negative transition

Query example :STATus:OPERation:NTRansition?
>1

The CAL bit is configured to NTR in the Operation Status NTR filter.

:STATus:OPERation:PTRansition



Description Determines whether a positive transition (PTR 0→1) in the Operation Status Condition register will set the corresponding event in the Operation Status Event register.

The mask values are the bit weights of the Operation Status PTR filters. See page 158 for details.

Syntax	:STATus:OPERation:PTRansition <NR1>			
Query Syntax	:STATus:OPERation:PTRansition?			
Parameter/ Return Parameter	<NR1>	Condition	<NR1>	Condition
	1	CAL	All other	Not used
	32	WTG	bits	
Example	:STATus:OPERation:PTRansition 32 Configures the WTG bit (Bit 5) in the Operation Status Condition register to set the corresponding bit in the Operation Status Enable register on a positive transition.			
Query example	:STATus:OPERation:PTRansition? >32 The WTG bit is configured to PTR in the Operation Status PTR filter.			

:STATus:CSUMmary:CONDition? → Query

Description	Returns the status of the CSummary Status Condition register. See page 156 for details.			
Query Syntax	:STATus:CSUMmary:CONDition?			
Return parameter	<NR1>	Condition	<NR1>	Condition
	1	CC	256	PRUN
	2	CR	All other	Not used
	4	CV	bits	
	8	CP		
Query example	:STATus:CSUMmary:CONDition? >1 Indicates the unit is in CC mode.			

:STATus:CSUMmary:ENABLE Set →
→ Query

Description	Sets which events are enabled in the CSummary Status Enable register. The mask values are the bit weights of the events. See page 156 for details.			
-------------	--	--	--	--

Syntax	:STATus:CSUMmary:ENABLE <NR1>			
Query Syntax	:STATus:CSUMmary:ENABLE?			
Parameter/ Return Parameter	<NR1>	Condition	<NR1>	Condition
	1	CC	256	PRUN
	2	CR	All other	Not used
	4	CV	bits	
	8	CP		
Example	:STATus:CSUMmary:ENABLE 1 Enables the CC bit in the CSummary Status Enable register.			
Query example	:STATus:CSUMmary:ENABLE? >1 Indicates that the CC bit is enabled in the CSummary Status Enable register.			

:STATus:CSUMmary[:EVENT]? → Query

Description	Returns the status of the CSummary Status Event register. The register is cleared upon reading. See page 156 for details.			
Query Syntax	:STATus:CSUMmary[:EVENT]?			
Return parameter	<NR1>	Condition	<NR1>	Condition
	1	CC	256	PRUN
	2	CR	All other	Not used
	4	CV	bits	
	8	CP		
Query example	:STATus:CSUMmary:EVENT? > 1 Indicates that the unit is in CC mode.			

:STATus:CSUMmary:NTRansition → Query

Description	Determines whether a negative transition (NTR 1→0) in the CSummary Status Condition register will set the corresponding event in the CSummary Status Event register.			
-------------	--	--	--	--

The mask values are the bit weights of the CSUMmary Status NTR filters. See page 156 for details.

Syntax :STATus:CSUMmary:NTRansition <NR1>

Query Syntax :STATus:CSUMmary:NTRansition?

Parameter/ Return Parameter	<NR1>	Condition	<NR1>	Condition
	1	CC	256	PRUN
	2	CR	All other bits	Not used
	4	CV		
	8	CP		


Example :STATus:CSUMmary:NTRansition 3

Configures the CC and CR bits (Bits 1, 2) in the CSUMmary Status Condition register to set the corresponding bits in the CSUMmary Status Enable register on a negative transition.

Query example :STATus:CSUMmary:NTRansition?
>3

The CC and CR bits are configured to NTR in the CSUMmary Status NTR filter.

:STATus:CSUMmary:PTRansition



Description Determines whether a positive transition (PTR 0→1) in the CSUMmary Status Condition register will set the corresponding event in the CSUMmary Status Event register.

The mask values are the bit weights of the CSUMmary Status PTR filters. See page 156 for details.

Syntax :STATus:CSUMmary:PTRansition <NR1>

Query Syntax :STATus:CSUMmary:PTRansition?

Parameter/ Return Parameter	<NR1>	Condition	<NR1>	Condition
	1	CC	256	PRUN
	2	CR	All other bits	Not used
	4	CV		
	8	CP		

Example :STATus:CSUMmary:PTRansition 12
Configures the CV and CP bits (Bits 3, 4) in the CSummary Status Condition register to set the corresponding bits in the CSummary Status Enable register on a positive transition.

Query example :STATus:CSUMmary:PTRansition?
>12
The CV and CP bits are configured to PTR in the CSummary Status PTR filter.

Status Registers

To program the PEL-3000 Series effectively, the Status Register structure needs to be understood. This chapter explains in detail the structure of the status registers.

Overview

The status registers are used to determine the status of the electronic load. The status registers maintain the status of the protection conditions, load conditions and channel conditions of the load modules.

The PEL-3000 series have a number of register groups:

CSummary Registers

Questionable Status Registers

Standard Event Status Registers


Status Byte Register

Service Request Generation Register

Each register group consists of a Condition, EVENT and ENABLE register. They also have PTR and NTR (positive and negative transition) filters.

The structure of the status registers is shown on the next page.

Status Registers

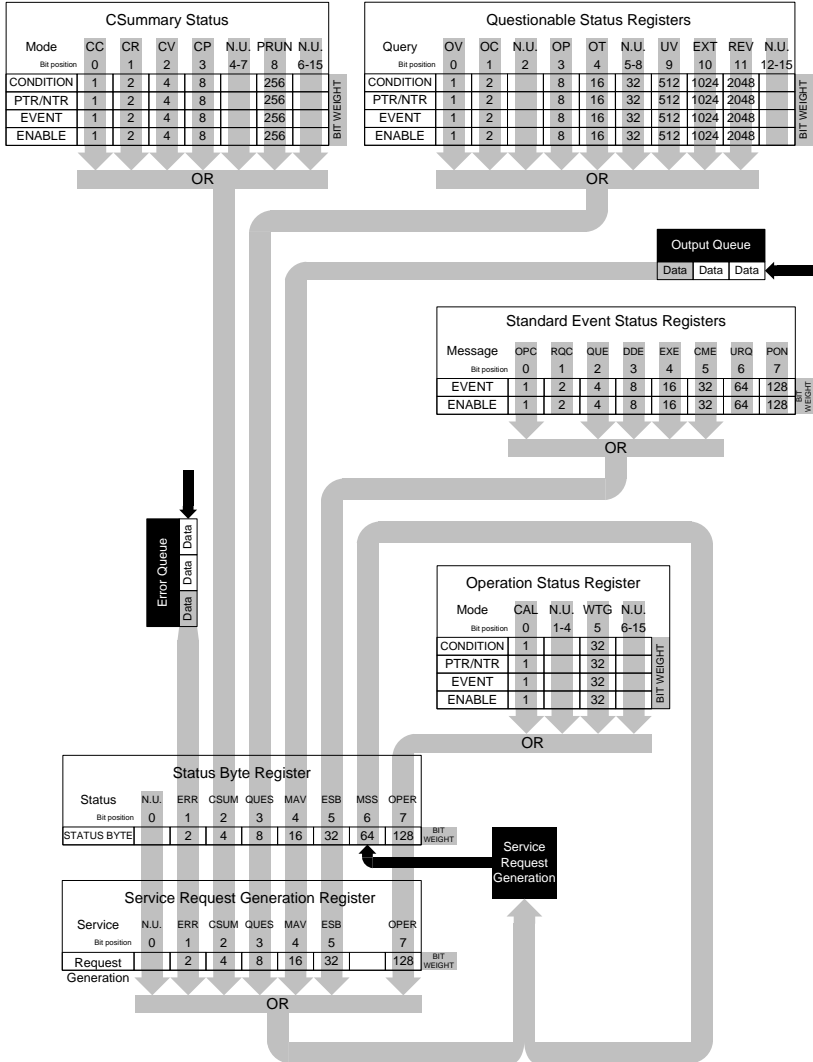

CSummary Status Registers

Overview

The CSummary Status registers indicate the current operation mode of the load generator.

CSummary Status Registers							
Bit Position	9-15	8	4-7	3	2	1	0
Condition	0	PRUN	0	CP	CV	CR	CP
PTR/NTR	0	PRUN	0	CP	CV	CR	CP
EVENT	0	PRUN	0	CP	CV	CR	CP
ENABLE	0	PRUN	0	CP	CV	CR	CP
Bit weight		256	16	8	4	2	1

Event Bits

CP: The unit has switched to CP mode.
 CR: The unit has switched to CR mode.
 CV: The unit has switched to CV mode.
 CP: The unit has switched to CP mode.
 PRUN: A program is running.

Condition Register

The condition register indicates the status of the electronic load. The condition register can only be changed by a change in the condition of the electronic load. Reading the condition register does not change the state of the condition register.

PTR/NTR Filters

The PTR/NTR (Positive/Negative transition) register determines the type of transition conditions that will trigger an event. Only the CSummary Status Register, Questionable Status Register and Operation Status Register can be transition programmed.

Event Register

The Event Register indicates if an event has been triggered according to the transition settings from the PTR/NTR Register.

Enable Register The Enable register determines which status event(s) are enabled. Any status events (CC, CV, CR, CP, PRUN) that are enabled will set the corresponding bit in the CSummary Event Register.

Questionable Status Registers

Overview The Questionable Status Registers will show if any faults or errors have occurred.

Questionable Status Register										
Bit Position	12-15	11	10	9	5-8	4	3	2	1	0
Condition	0	REV	EXT	UV	0	OT	OP	0	OC	OV
PTR/NTR	0	REV	EXT	UV	0	OT	OP	0	OC	OV
EVENT	0	REV	EXT	UV	0	OT	OP	0	OC	OV
ENABLE	0	REV	EXT	UV	0	OT	OP	0	OC	OV
Bit weight		2048	1024	512		16	8	4	2	1

Events Bits

- OV: Over voltage condition occurred.
- OC: Over current condition occurred.
- OP: Over power condition occurred.
- OT: Over temperature condition occurred.
- UV: Under voltage condition occurred.
- EXT: External problem occurred. (Same a Para alarm event: UnReg, R.OCP, OHP condition occurred.)
- REV: A reverse voltage condition has occurred.

Condition Register The condition register indicates the status of the protection systems. The condition register can only be changed by a change in the condition of the protection systems. Reading the condition register does not change the state of the condition register.

- PTR/NTR Filters** The PTR/NTR (Positive/Negative transition) register determines the type of transition conditions that will trigger an event. Only the CSummary Status Register, Questionable Status Register and Operation Status Register can be transition programmed.
- Event Register** The Event Register indicates if an event has been triggered according to the transition settings from the PTR/NTR Register.
- Enable Register** The Enable register determines which status event(s) are enabled. Any status events (OV, OC, OP, OT, UV, EXT or REV) that are enabled will set the corresponding bit in the Questionable Event Register.

Operation Status Registers

Overview The Operation Status Registers will show the operating state of electronic load (waiting for a trigger or in calibration mode).

Operation Status Registers			
Bit Position	5	1-4	0
Condition	WTG	0	CAL
PTR/NTR	WTG	0	CAL
EVENT	WTG	0	CAL
ENABLE	WTG	0	CAL
Bit weight	32	1	

Events Bits

CAL: Indicates that the unit is currently in calibration mode.

WTG: Indicates that the unit is waiting for a trigger.

- Condition Register The condition register indicates the operating state of the unit. The condition register can only be changed by a change in the condition of operating state. Reading the condition register does not change the state of the condition register.

- PTR/NTR Filters The PTR/NTR (Positive/Negative transition) register determines the type of transition conditions that will trigger an event. Only the CSummary Status Register, Questionable Status Register and Operation Status Register can be transition programmed.

- Event Register The Event Register indicates if an event has been triggered according to the transition settings from the PTR/NTR Register.

- Enable Register The Enable register determines which status event(s) are enabled. Any status events (CAL or WTG) that are enabled will set the corresponding bit in the Operation Event Register.

Standard Event Status Registers

- Overview The Standard Event Status Registers indicate any programming errors that occur. The Standard Event Status Register group comprises of the Event and Enable registers.

Standard Event Status Registers								
Bit Position	7	6	5	4	3	2	1	0
EVENT	PON	URQ	CME	EXE	DDE	QUE	RQC	OPC
ENABLE	PON	URQ	CME	EXE	DDE	QUE	RQC	OPC
Bit weight	128	64	32	16	8	4	2	1

Events Bits	<p>OPC: The operation complete bit is set when all selected pending operations are complete. This bit is set in response to the *OPC command.</p> <p>RQC: Not used.</p> <p>QUE: The query error bit is set when there is an error reading the output queue. This can be caused by trying to read the output queue when there is no data in it.</p> <p>DDE: The Device Dependent Error indicates a memory error/lost memory or failure of the self-test.</p> <p>EXE: The Execution bit indicates an execution error due to one of the following:</p> <ul style="list-style-type: none">-Illegal command parameter-Parameter out of range-Invalid parameter-Command didn't execute due to an overriding operation condition. <p>CME: The Command Error bit can be set when a syntax error has occurred, an unidentifiable header is received or when a <GET> command is received within a program message. (Group Execute Trigger) as defined in IEEE 488.1.</p> <p>URQ: Not used.</p> <p>PON: Not used.</p>
Event Register	<p>The Event Register will be set to 0 when read.</p>
Enable Register	<p>The Enable Register determines which events will set the ESB Bit (bit 5) in the Status Byte Register.</p>

Status Byte Register

Overview

The Status Byte register consolidates the status events of all the status registers. The Status Byte register can be read with the *STB? query or a serial poll and can be cleared with the *CLS command.

Status Byte Register								
Bit Position	7	6	5	4	3	2	1	0
Condition	OPER	MSS	ESB	MAV	QUES	CSUM	ERR	0
Bit weight	128	64	32	16	8	4	2	1

Status Bits

ERR: The ERR bit is set when there is a message in the error queue.

CSUM: The CSUM bit is set when an event has occurred in the CSummary Status Register group.

QUES: The QUES bit is set when an event has occurred in the Questionable Status Register group.

MAV: The MAV bit is set when there is outstanding data in the Output Queue.

ESB: The Event Status bit is set if an enabled event in the Standard Event Status Register group has occurred.

MSS & RQS: The Master Summary Status is used with the *STB? query. When the *STB? query is read, the MSS bit is not cleared. The Request Service bit is cleared when it is polled during a serial poll.

OPER: The OPER bit is set when if an enabled event in the Operation Status Register has occurred.

Service Request Register

Overview

The Service Request Generation Register determines which events in the Status Byte Register will generate Service Requests. It is essentially the Status Byte Enable Register. The bit events are the same as the Status Byte Register, minus the MSS/RQS bit.

Service Request Generation Register (Status Byte Enable)

Bit Position	7	6	5	4	3	2	1	0
Condition	OPER	0	ESB	MAV	QUES	CSUM	ERR	0
Bit weight	128	64	32	16	8	4	2	1

Error Messages

The following error messages may be encountered when reading the error queue.

Error Code and string	Description
Command Errors	
0 NoError	No error
-100 Command Error	This is the generic syntax error for devices that cannot detect more specific errors.
-101 Invalid character	A syntactic element contains a character which is invalid for that type.
-102 Syntax error	An unrecognized command or data type was encountered.
-103 Invalid separator	The parser was expecting a separator and encountered an illegal character.
-104 Data type error	The parser recognized a data element different than the one allowed.
-105 GET not allowed	A Group Execute Trigger was received within a program message.
-108 Parameter not allowed	More parameters were received than expected for the header.
-109 Missing parameter	Fewer parameters were received than required for the header.
-110 Command header error	An error was detected in the header.

-111 Header separator error	A character which is not a legal header separator was encountered while parsing the header.
-112 Program mnemonic too long	The header contains more than twelve characters.
-113 Undefined header	The header is syntactically correct, but it is undefined for this specific device.
-114 Header suffix out of range	The value of a numeric suffix attached to a program mnemonic.
-115 Unexpected number of parameters	The number of parameters received does not correspond to the number of parameters expected.
-120 Numeric data error	This error is generated when parsing a data element which appears to be numeric, including the nondecimal numeric types.
-121 Invalid character in number	An invalid character for the data type being parsed was encountered.
-123 Exponent too large	The magnitude of the exponent was larger than 32000.
-124 Too many digits	The mantissa of a decimal numeric data element contained more than 255 digits excluding leading zeros.
-128 Numeric data not allowed	A legal numeric data element was received, but the device does not accept one in this position for the header
-130 Suffix error	This error, as well as errors -131 through -139, are generated when parsing a suffix.

-131 Invalid suffix	The suffix does not follow the syntax described in IEEE 488.2 or the suffix is inappropriate for this device.
-134 Suffix too long	The suffix contained more than 12 characters.
-138 Suffix not allowed	A suffix was encountered after a numeric element which does not allow suffixes.
-140 Character data error	This error is generated when parsing a character data element.
-141 Invalid character data	Either the character data element contains an invalid character or the particular element received is not valid for the header.
-144 Character data too long	The character data element contains more than twelve characters
-148 Character data not allowed	A legal character data element was encountered where prohibited by the device.
-150 String data error	This error is generated when parsing a string data element.
-151 Invalid string data	A string data element was expected, but was invalid for some reason.
-158 String data not allowed	A string data element was encountered but was not allowed by the device at this point in parsing.
-160 Block data error	This error is generated when parsing a block data element.
-161 Invalid block data	A block data element was expected, but was invalid for some reason.

-168 Block data not allowed	A legal block data element was encountered but was not allowed by the device at this point in parsing.
-170 Expression error	This error is generated when parsing an expression data element.
-171 Invalid expression	The expression data element was invalid.
-178 Expression data not allowed	A legal expression data was encountered but was not allowed by the device at this point in parsing.
-180 Macro error	This error is generated when defining a macro or executing a macro.
-181 Invalid outside macro definition	Indicates that a macro parameter placeholder (\$<number>) was encountered outside of a macro definition.
-183 Invalid inside macro definition	Indicates that the program message unit sequence, sent with a *DDT or *DMC command, is syntactically invalid.
-184 Macro parameter error	Indicates that a command inside the macro definition had the wrong number or type of parameters.

Execution Errors

-200 Execution error	This is the generic syntax error for devices that cannot detect more specific errors. This code indicates only that an Execution Error as defined in IEEE 488.2 has occurred.
-201 Invalid while in local	Indicates that a command is not executable while the device is in local due to a hard local control
-202 Settings lost due to rtl	Indicates that a setting associated with a hard local control was lost when the device changed to LOCS from REMS or to LWLS from RWLS.
-203 Command protected	Indicates that a legal password-protected program command or query could not be executed because the command was disabled.
-210 Trigger error	
-211 Trigger ignored	Indicates that a GET, *TRG, or triggering signal was received and recognized by the device but was ignored because of device timing considerations.
-212 Arm ignored	Indicates that an arming signal was received and recognized by the device but was ignored.
-213 Init ignored	Indicates that a request for a measurement initiation was ignored as another measurement was already in progress.

-214 Trigger deadlock	Indicates that the trigger source for the initiation of a measurement is set to GET and subsequent measurement query is received. The measurement cannot be started until a GET is received, but the GET would cause an INTERRUPTED error.
-215 Arm deadlock	Indicates that the arm source for the initiation of a measurement is set to GET and subsequent measurement query is received. The measurement cannot be started until a GET is received, but the GET would cause an INTERRUPTED error.
-220 Parameter error	Indicates that a program data element related error occurred.
-221 Settings conflict	Indicates that a legal program data element was parsed but could not be executed due to the current device state.
-222 Data out of range	Indicates that a legal program data element was parsed but could not be executed because the interpreted value was outside the legal range as defined by the device.
-223 Too much data	Indicates that a legal program data element of block, expression, or string type was received that contained more data than the device could handle due to memory or related device-specific requirements.

-224 Illegal parameter value	Used where an exact value, from a list of possibilities, was expected.
-225 Out of memory.	The device has insufficient memory to perform the requested operation.
-226 Lists not same length.	Attempted to use LIST structure having individual LIST's of unequal lengths.
-230 Data corrupt or stale	Possibly invalid data; new reading started but not completed since last access.
-231 Data questionable	Indicates that measurement accuracy is suspect.
-232 Invalid format	Indicates that a legal program data element was parsed but could not be executed because the data format or structure is inappropriate.
-233 Invalid version	Indicates that a legal program data element was parsed but could not be executed because the version of the data is incorrect to the device.
-240 Hardware error	Indicates that a legal program command or query could not be executed because of a hardware problem in the device.
-241 Hardware missing	Indicates that a legal program command or query could not be executed because of missing device hardware.
-250 Mass storage error	Indicates that a mass storage error occurred.

-251 Missing mass storage	Indicates that a legal program command or query could not be executed because of missing mass storage.
-252 Missing media	Indicates that a legal program command or query could not be executed because of a missing media.
-253 Corrupt media	Indicates that a legal program command or query could not be executed because of corrupt media.
-254 Media full	Indicates that a legal program command or query could not be executed because the media was full.
-255 Directory full	Indicates that a legal program command or query could not be executed because the media directory was full.
-256 File name not found	Indicates that a legal program command or query could not be executed because the file name on the device media was not found.
-257 File name error	Indicates that a legal program command or query could not be executed because the file name on the device media was in error.
-258 Media protected	Indicates that a legal program command or query could not be executed because the media was protected.
-260 Expression error	Indicates that a expression program data element related error occurred.

-261 Math error in expression	Indicates that a syntactically legal expression program data element could not be executed due to a math error.
-270 Macro error	Indicates that a macro-related execution error occurred.
-271 Macro syntax error	Indicates that that a syntactically legal macro program data sequence, according to IEEE 488.2 could not be executed due to a syntax error within the macro definition.
-272 Macro execution error	Indicates that a syntactically legal macro program data sequence could not be executed due to some error in the macro definition.
-273 Illegal macro label	Indicates that the macro label defined in the *DMC command was a legal string syntax, but could not be accepted by the device.
-274 Macro parameter error	Indicates that the macro definition improperly used a macro parameter placeholder.
-275 Macro definition too long	Indicates that a syntactically legal macro program data sequence could not be executed because the string or block contents were too long for the device to handle.
-276 Macro recursion error	Indicates that a syntactically legal macro program data sequence could not be executed because the device found it to be recursive.

-
- | | |
|-------------------------------------|---|
| -277 Macro redefinition not allowed | Indicates that a syntactically legal macro label in the *DMC command could not be executed because the macro label was already defined. |
| -278 Macro header not found | Indicates that a syntactically legal macro label in the *GMC? query could not be executed because the header was not previously defined. |
| -280 Program error | Indicates that a downloaded program-related execution error occurred. |
| -281 Cannot create program | Indicates that an attempt to create a program was unsuccessful. A reason for the failure might include not enough memory. |
| -282 Illegal program name | The name used to reference a program was invalid. |
| -283 Illegal variable name | An attempt was made to reference a nonexistent variable in a program. |
| -284 Program currently running | Certain operations dealing with programs may be illegal while the program is running. |
| -285 Program syntax error | Indicates that a syntax error appears in a downloaded program. |
| -286 Program runtime error | |
| -290 Memory use error | Indicates that a user request has directly or indirectly caused an error related to memory or <data_handle>s, this is not the same as "bad" memory. |
| -291 Out of memory | |

- 292 Referenced name does not exist
- 293 Referenced name already exists
- 294 Incompatible type Indicates that the type or structure of a memory item is inadequate.

Device Specific Errors

- 300 Device-specific error This is the generic device-dependent error for devices that cannot detect more specific errors.
- 310 System error Indicates that some error, termed "system error" by the device, has occurred.
- 311 Memory error Indicates some physical fault in the device's memory, such as parity error.
- 312 PUD memory lost Indicates that the protected user data saved by the *PUD command has been lost.
- 313 Calibration memory lost Indicates that nonvolatile calibration data used by the *CAL? command has been lost.
- 314 Save/recall memory lost Indicates that the nonvolatile data saved by the *SAV? command has been lost.
- 315 Configuration memory lost Indicates that nonvolatile configuration data saved by the device has been lost.

-320 Storage fault	[Indicates that the firmware detected a fault when using data storage. This error is not an indication of physical damage or failure of any mass storage element.
-321 Out of memory	An internal operation needed more memory than was available.
-330 Self-test failed	
-340 Calibration failed	
-350 Queue overflow	A specific code entered into the queue in lieu of the code that caused the error. This code indicates that there is no room in the queue and an error occurred but was not recorded.
-360 Communication error	This is the generic communication error.
-361 Parity error in program message	Parity bit not correct when data received.
-362 Framing error in program message	A stop bit was not detected when data was received.
-363 Input buffer overrun	Software or hardware input buffer on serial port overflows with data caused by improper or nonexistent pacing.
-365 Time out error	This is a generic device-dependent error.

Query Errors

-400 Query error	This is the generic query error.
-410 Query INTERRUPTED	Indicates that a condition causing an INTERRUPTED Query error occurred.

-420 Query UNTERMINATED	Indicates that a condition causing an UNTERMINATED Query error occurred.
-430 Query DEADLOCKED	Indicates that a condition causing an DEADLOCKED Query error occurred.
-440 Query UNTERMINATED after indefinite response	Indicates that a query was received in the same program message after a query requesting an indefinite response was executed

Power On Event Commands

-500 Power on	The instrument has detected an off to on transition in its power supply.
---------------	--

User Request Event

-600 User request	The instrument has detected the activation of a user request local control.
-------------------	---

Request Control Event

-700 Request control	The instrument requested to become the active IEEE 488.1 controller-in-charge.
----------------------	--

Operation Complete Event

-800 Operation complete	The instrument has completed all selected pending operations in accordance with the IEEE 488.2 synchronization protocol.
-------------------------	--